

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate www.vevor.com/support

COMMODE

MODEL:FBL730211

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

VEVOR[®]

TOUGH TOOLS, HALF PRICE

COMMODE

MODEL:FBL730211



NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

Technical Support and E-Warranty Certificate
www.vevor.com/support

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

WARNING:

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

Physiotherapist

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to standing position, place your hands on the rails firmly, and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).














IMPORTANT

1. Don't exceed the weight capacity max.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

SAVE THESE INSTRUCTION

PART LIST


When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.

NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Leg Tube	4	⑧		Short Backrest Tube	1
②		Left Front Main Frame	1	⑨		Long Backrest Tube	1
③		Left Rear Main Frame	1	⑩		Right Rear Main Frame	1
④		Armrest Tube	2	⑪		Right Front Main Frame	1
⑤		Seat	1	⑫		Paper Towel Holder	1
⑥		Pail & Splash Shield & Lid	1	⑬		Foot Mats (*Gifts)	2
⑦		Flat Knob	4				


PRODUCT PAREMETERS

Model	FBL730211
Seat Measures (L×W)	440×400mm / 17.3"×15.7"
Seat Height	495-645mm / 20.3"-25.4"
Seat Rated Load	159kg / 350lbs


INSTALLATION AND OPERATION INSTRUCTIONS

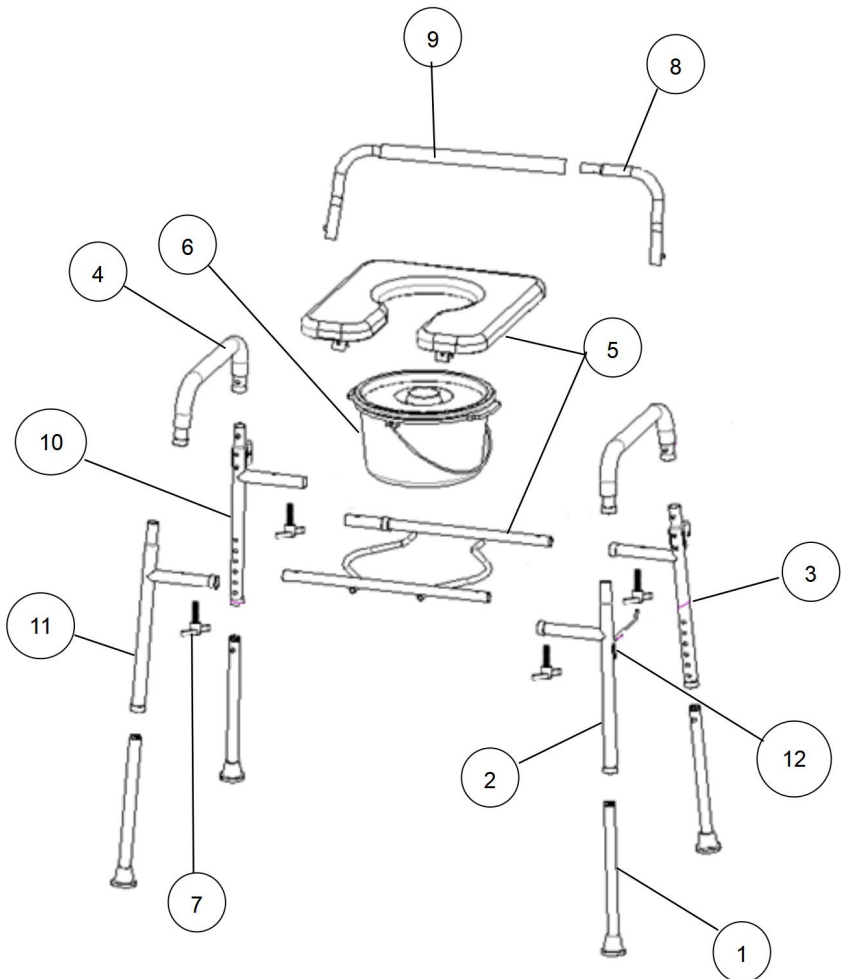


1. As shown in the figure, the four legs① are installed into the left front main frame②, the left rear main frame③, the right rear main frame⑩ and the right front main frame⑪ in turn.

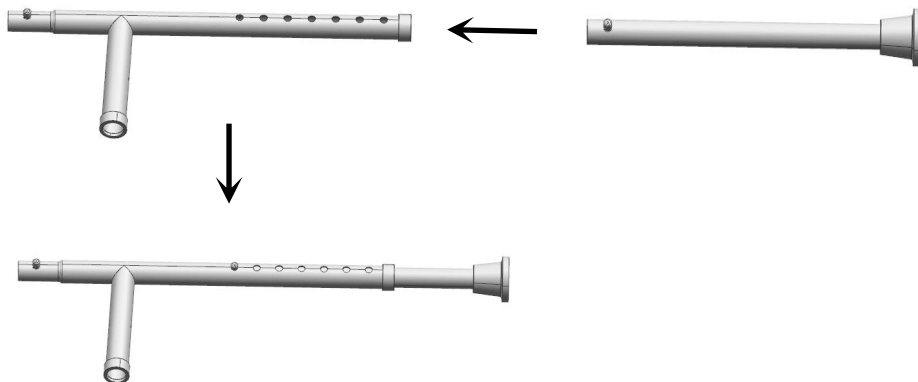


2. As shown in the figure, the assembled left front main frame ②, left rear main frame ③, right rear main frame ⑩, and right front main frame are put into the armrest tube ④ respectively, so that the marbles of each main frame eject normally.

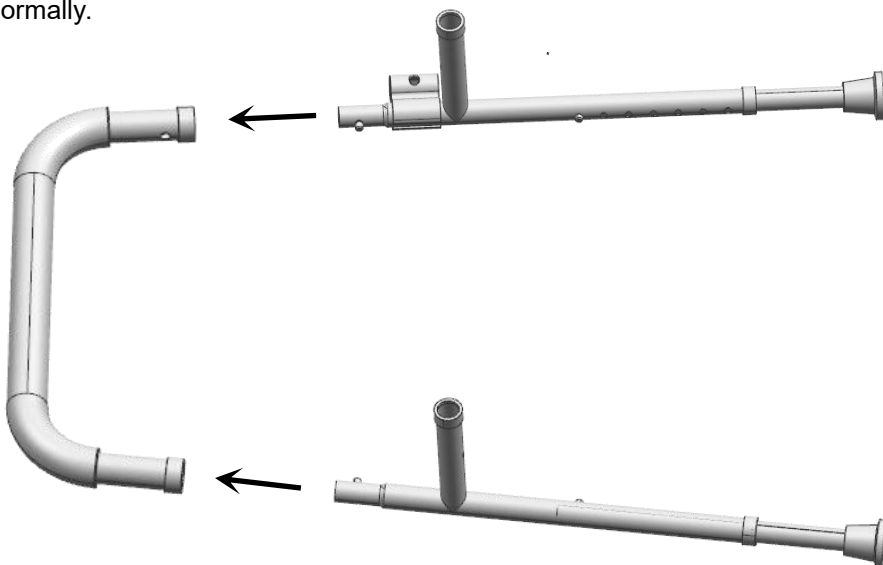


3. As shown in the figure, insert the assembled left and right main frames in line with the tube openings of the seat frame ⑤ (be careful not to install the seat frame and main frame in the front and rear directions in reverse).

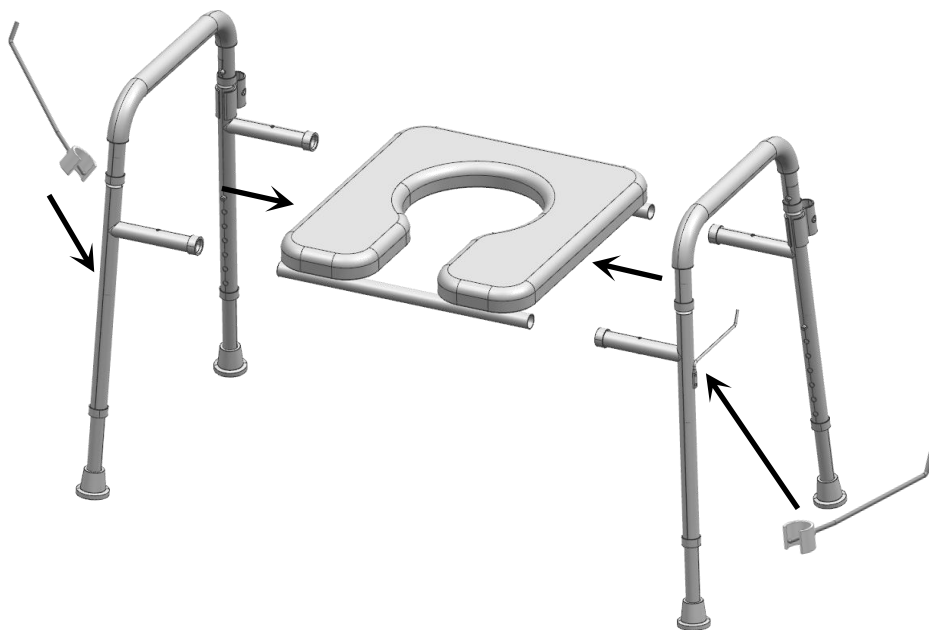


4. As shown in the figure, install the paper towel holder card ⑫ on the corresponding position of the left front main frame ② or right front main frame according to the usage habits.



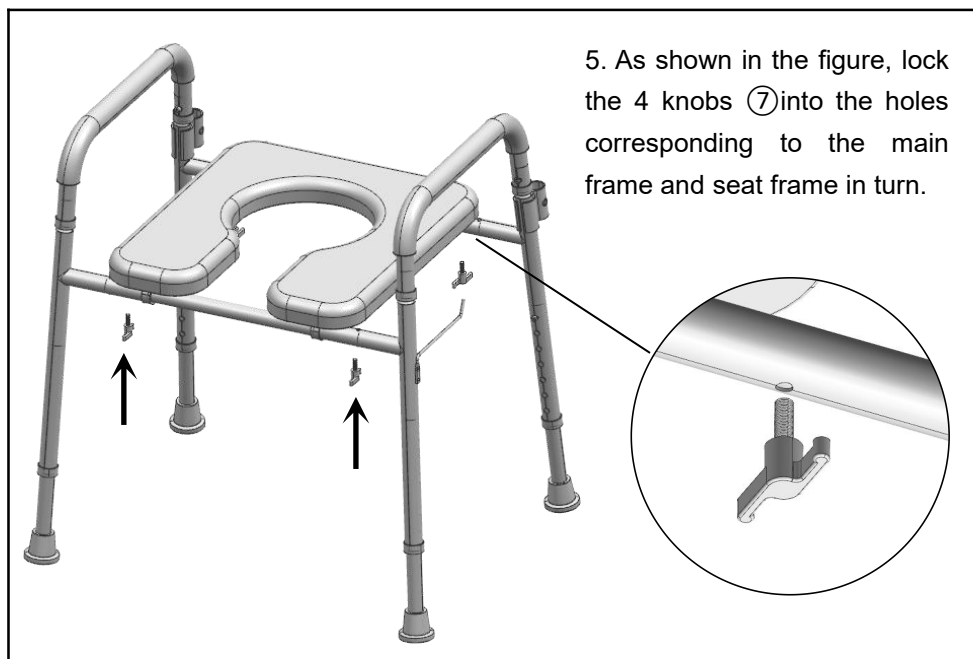


6. As shown in the figure, insert the short backrest tube ⑧ and the long backrest tube ⑨ mouth alignment, so that the marbles pop up normally (Note: Try to pull the two tubes apart by hand to confirm whether the two tubes are assembled).

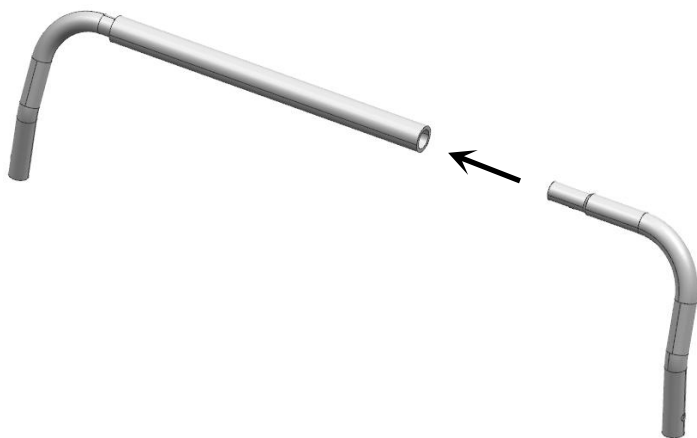

7. Insert the entire assembled backrest tube into the short tubes on either side of the rear main frame as shown.



8. As shown, lift the seat plate upwards and place the pail into the seat frame.

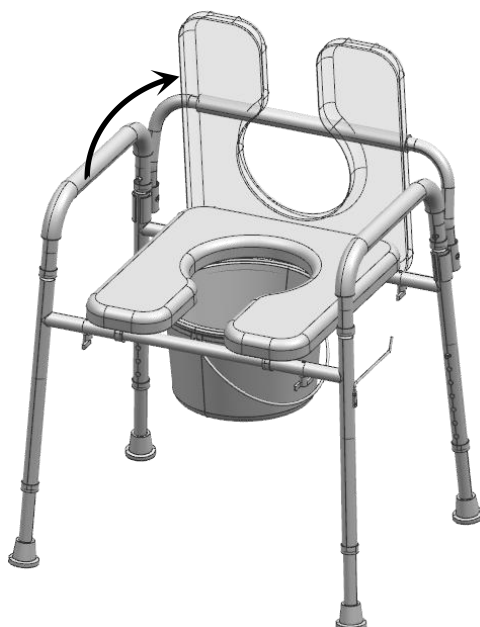

Zhongshan Bliss Medical Instrument Co., Ltd

Address: 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd
Unit 5 Albert Edward House,
The Pavilions Preston, United Kingdom
pooledas123@gmail.com
01772418127



SHUNSHUN GmbH
Römeräcker 9 Z2021,76351
Linkenheim-Hochstetten, Germany
euvertreter@gmail.com
+49 1727041930

Made In China

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate

www.vevor.com/support

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate www.vevor.com/support

COMMODE

MODEL:FBL730211

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

VEVOR®

TOUGH TOOLS, HALF PRICE

COMMODE

MODEL:FBL730211



NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

Technical Support and E-Warranty Certificate
www.vevor.com/support

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

WARNING:

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

Physiotherapist

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to standing position, place your hands on the rails firmly, and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).














IMPORTANT

1. Don't exceed the weight capacity max.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

SAVE THESE INSTRUCTION

PART LIST


When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.

NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Leg Tube	4	⑧		Short Backrest Tube	1
②		Left Front Main Frame	1	⑨		Long Backrest Tube	1
③		Left Rear Main Frame	1	⑩		Right Rear Main Frame	1
④		Armrest Tube	2	⑪		Right Front Main Frame	1
⑤		Seat	1	⑫		Paper Towel Holder	1
⑥		Pail & Splash Shield & Lid	1	⑬		Foot Mats (*Gifts)	2
⑦		Flat Knob	4				


PRODUCT PAREMETERS

Model	FBL730211
Seat Measures (L×W)	440×400mm / 17.3"×15.7"
Seat Height	495-645mm / 20.3"-25.4"
Seat Rated Load	159kg / 350lbs


INSTALLATION AND OPERATION INSTRUCTIONS

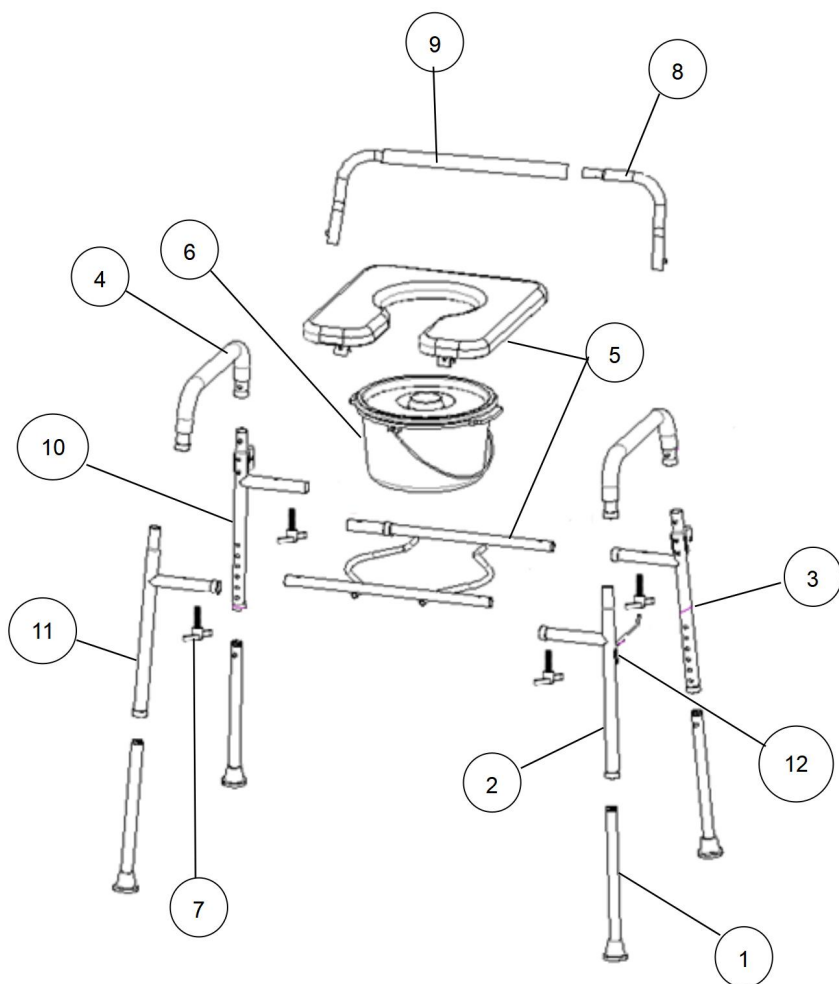


1. As shown in the figure, the four legs① are installed into the left front main frame②, the left rear main frame③, the right rear main frame⑩ and the right front main frame⑪ in turn.

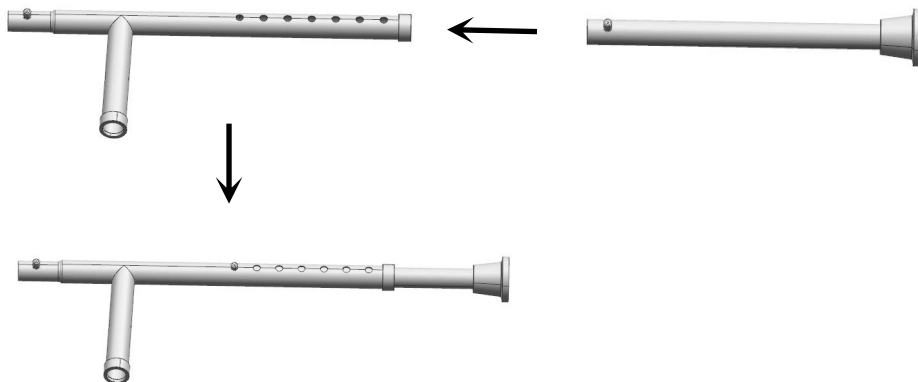


2. As shown in the figure, the assembled left front main frame ②, left rear main frame ③, right rear main frame ⑩, and right front main frame are put into the armrest tube ④ respectively, so that the marbles of each main frame eject normally.

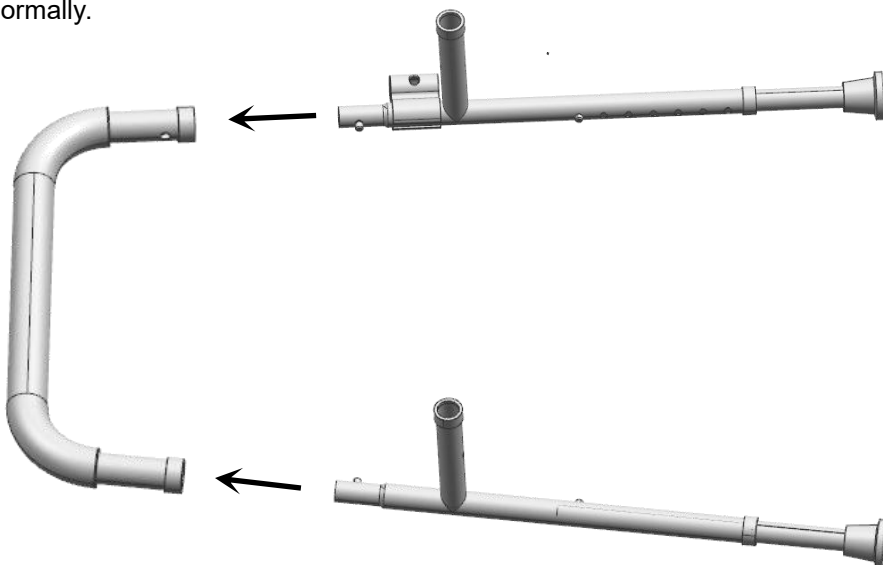


3. As shown in the figure, insert the assembled left and right main frames in line with the tube openings of the seat frame ⑤ (be careful not to install the seat frame and main frame in the front and rear directions in reverse).

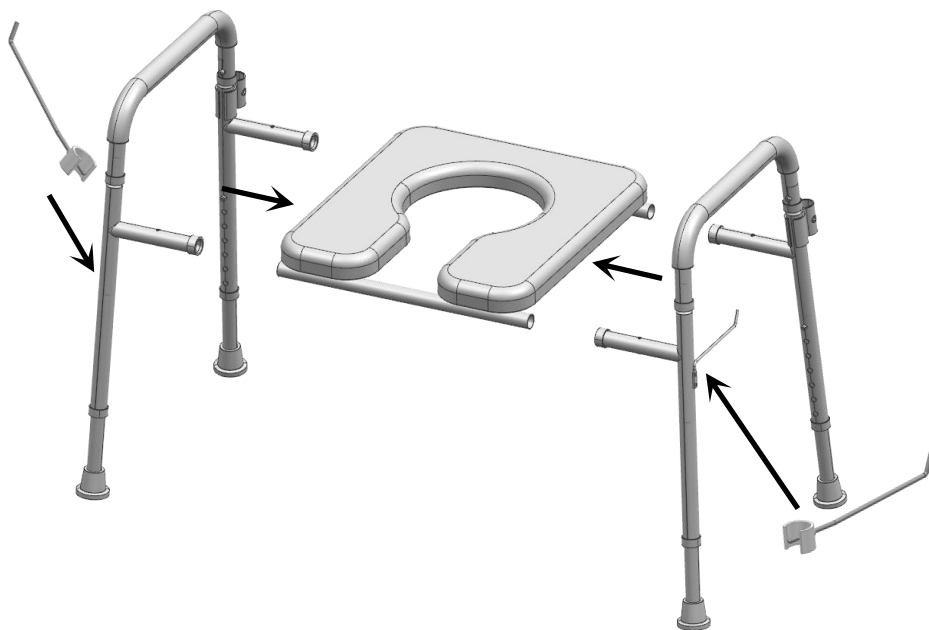


4. As shown in the figure, install the paper towel holder card ⑫ on the corresponding position of the left front main frame ② or right front main frame according to the usage habits.



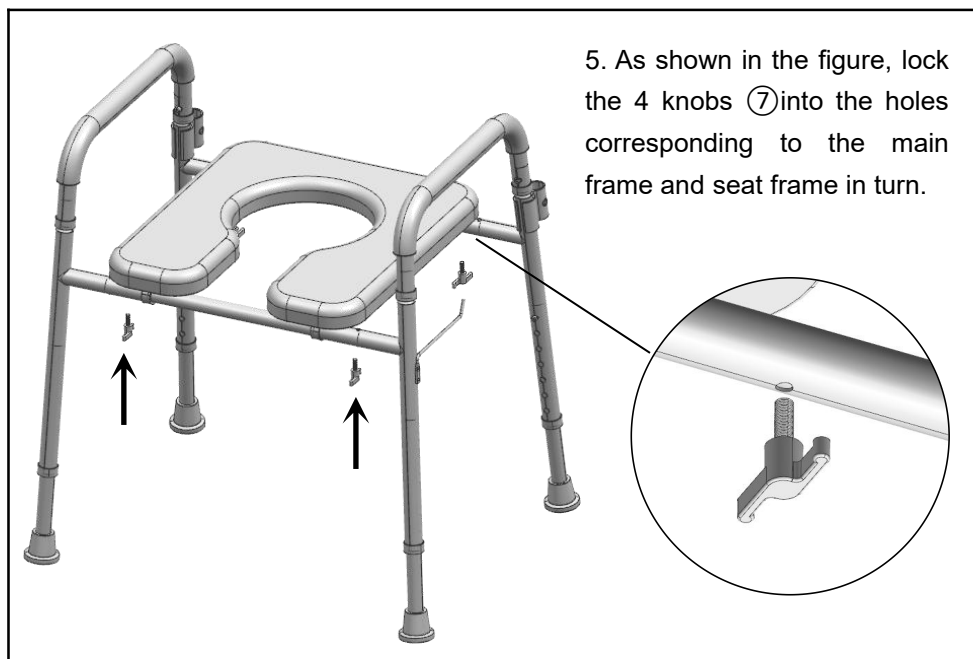


6. As shown in the figure, insert the short backrest tube ⑧ and the long backrest tube ⑨ mouth alignment, so that the marbles pop up normally (Note: Try to pull the two tubes apart by hand to confirm whether the two tubes are assembled).

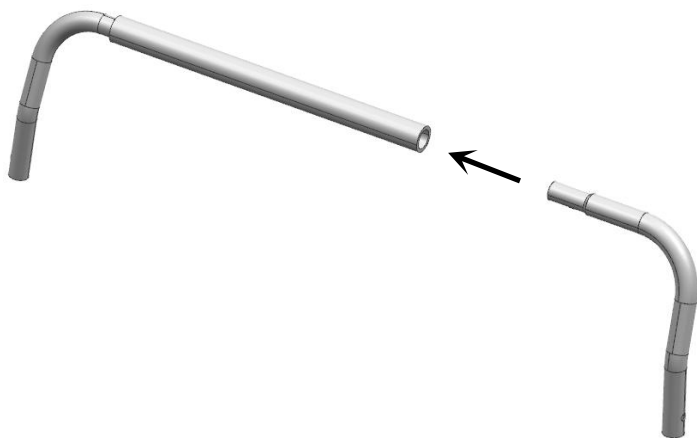

7. Insert the entire assembled backrest tube into the short tubes on either side of the rear main frame as shown.



8. As shown, lift the seat plate upwards and place the pail into the seat frame.

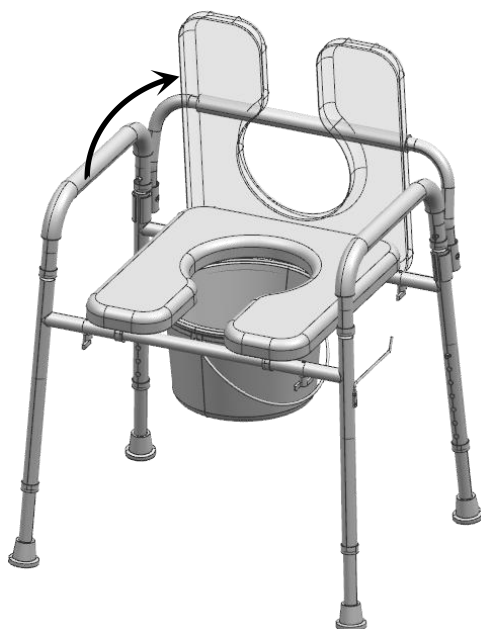

Zhongshan Bliss Medical Instrument Co., Ltd

Address: 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd
Unit 5 Albert Edward House,
The Pavilions Preston, United Kingdom
pooledas123@gmail.com
01772418127



SHUNSHUN GmbH
Römeräcker 9 Z2021,76351
Linkenheim-Hochstetten, Germany
euvertreter@gmail.com
+49 1727041930

Made In China

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate

www.vevor.com/support

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate www.vevor.com/support

COMMODE

MODEL:FBL730211

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

VEVOR[®]

TOUGH TOOLS, HALF PRICE

COMMODE

MODEL:FBL730211



NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

Technical Support and E-Warranty Certificate
www.vevor.com/support

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

WARNING:

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

Physiotherapist

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to standing position, place your hands on the rails firmly, and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).














IMPORTANT

1. Don't exceed the weight capacity max.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

SAVE THESE INSTRUCTION

PART LIST


When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.

NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Leg Tube	4	⑧		Short Backrest Tube	1
②		Left Front Main Frame	1	⑨		Long Backrest Tube	1
③		Left Rear Main Frame	1	⑩		Right Rear Main Frame	1
④		Armrest Tube	2	⑪		Right Front Main Frame	1
⑤		Seat	1	⑫		Paper Towel Holder	1
⑥		Pail & Splash Shield & Lid	1	⑬		Foot Mats (*Gifts)	2
⑦		Flat Knob	4				


PRODUCT PAREMETERS

Model	FBL730211
Seat Measures (L×W)	440×400mm / 17.3"×15.7"
Seat Height	495-645mm / 20.3"-25.4"
Seat Rated Load	159kg / 350lbs


INSTALLATION AND OPERATION INSTRUCTIONS

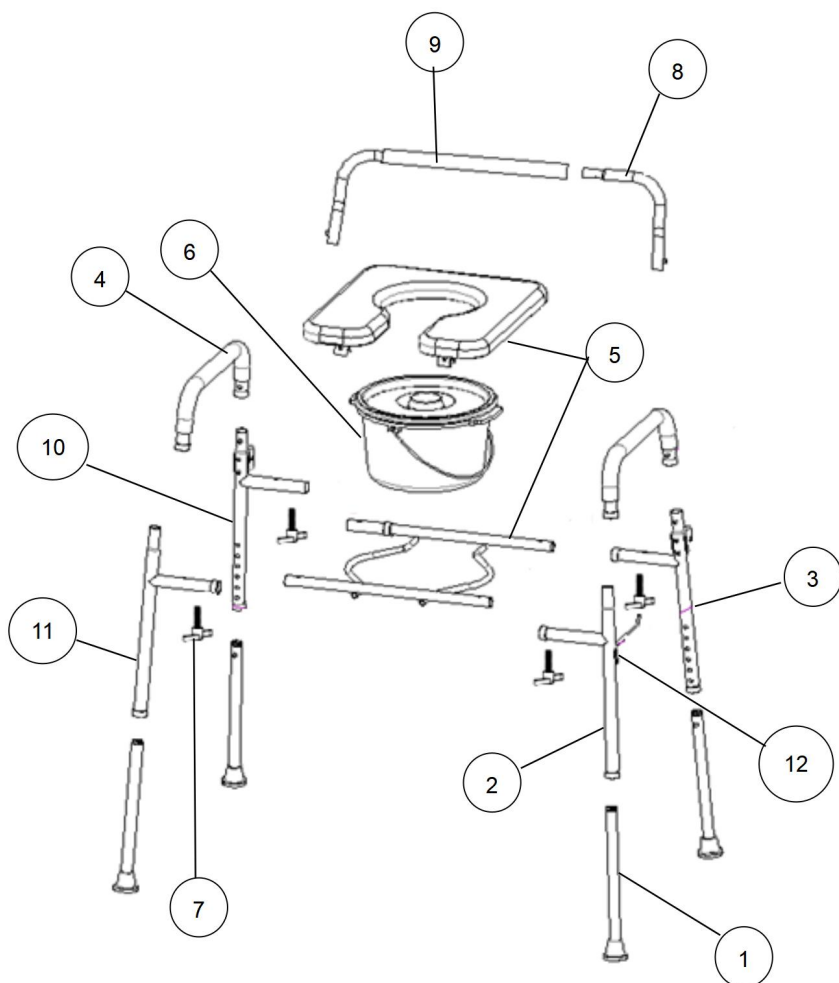


1. As shown in the figure, the four legs① are installed into the left front main frame②, the left rear main frame③, the right rear main frame⑩ and the right front main frame⑪ in turn.

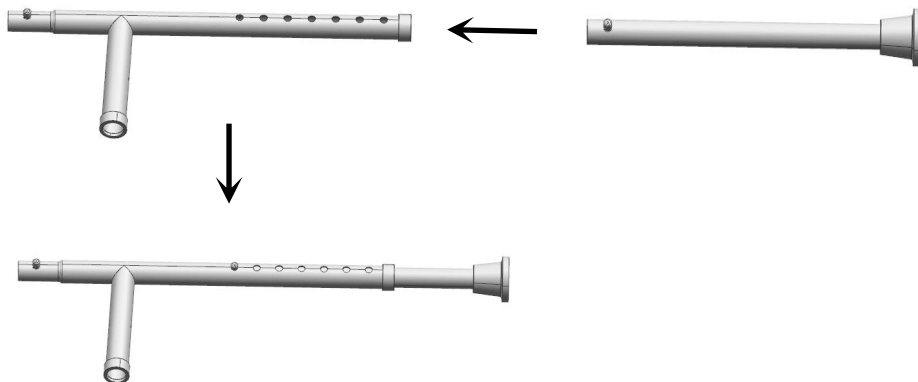


2. As shown in the figure, the assembled left front main frame ②, left rear main frame ③, right rear main frame ⑩, and right front main frame are put into the armrest tube ④ respectively, so that the marbles of each main frame eject normally.

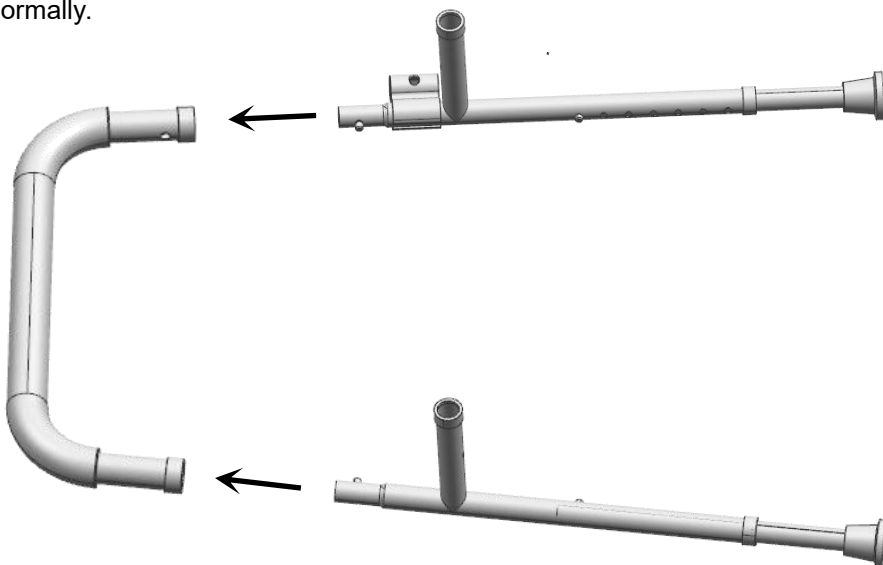


3. As shown in the figure, insert the assembled left and right main frames in line with the tube openings of the seat frame ⑤ (be careful not to install the seat frame and main frame in the front and rear directions in reverse).

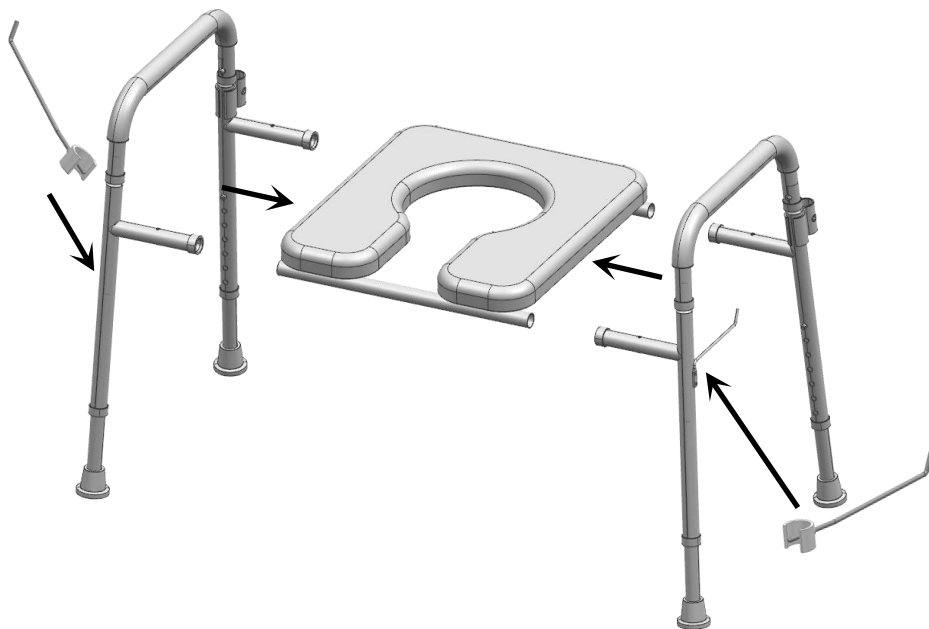


4. As shown in the figure, install the paper towel holder card ⑫ on the corresponding position of the left front main frame ② or right front main frame according to the usage habits.



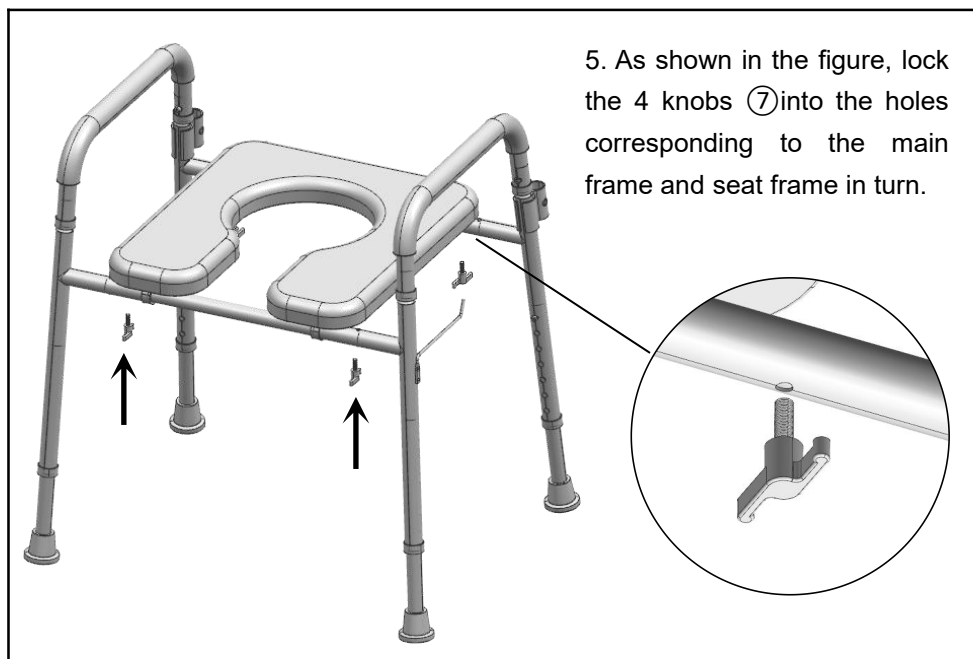


6. As shown in the figure, insert the short backrest tube ⑧ and the long backrest tube ⑨ mouth alignment, so that the marbles pop up normally (Note: Try to pull the two tubes apart by hand to confirm whether the two tubes are assembled).

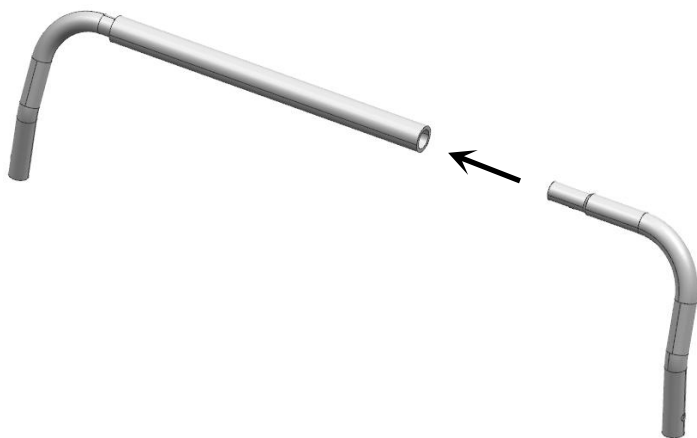

7. Insert the entire assembled backrest tube into the short tubes on either side of the rear main frame as shown.



8. As shown, lift the seat plate upwards and place the pail into the seat frame.

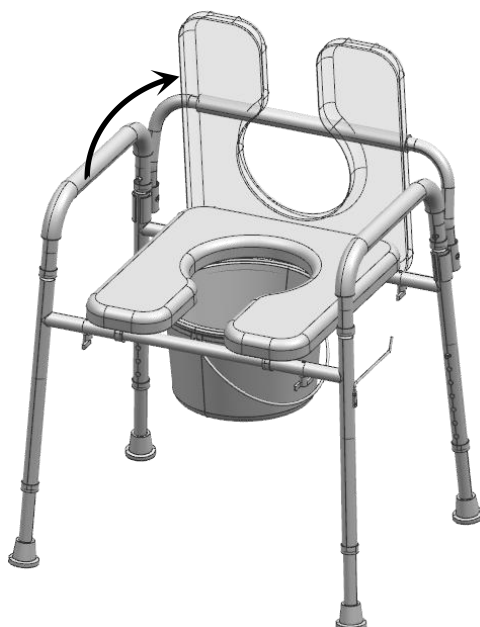

Zhongshan Bliss Medical Instrument Co., Ltd

Address: 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd
Unit 5 Albert Edward House,
The Pavilions Preston, United Kingdom
pooledas123@gmail.com
01772418127



SHUNSHUN GmbH
Römeräcker 9 Z2021,76351
Linkenheim-Hochstetten, Germany
euvertreter@gmail.com
+49 1727041930

Made In China

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate

www.vevor.com/support

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate www.vevor.com/support

COMMODE

MODEL:FBL730211

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

VEVOR®

TOUGH TOOLS, HALF PRICE

COMMODE

MODEL:FBL730211



NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

Technical Support and E-Warranty Certificate
www.vevor.com/support

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

WARNING:

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

Physiotherapist

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to standing position, place your hands on the rails firmly, and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).














IMPORTANT

1. Don't exceed the weight capacity max.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

SAVE THESE INSTRUCTION

PART LIST


When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.

NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Leg Tube	4	⑧		Short Backrest Tube	1
②		Left Front Main Frame	1	⑨		Long Backrest Tube	1
③		Left Rear Main Frame	1	⑩		Right Rear Main Frame	1
④		Armrest Tube	2	⑪		Right Front Main Frame	1
⑤		Seat	1	⑫		Paper Towel Holder	1
⑥		Pail & Splash Shield & Lid	1	⑬		Foot Mats (*Gifts)	2
⑦		Flat Knob	4				


PRODUCT PAREMETERS

Model	FBL730211
Seat Measures (L×W)	440×400mm / 17.3"×15.7"
Seat Height	495-645mm / 20.3"-25.4"
Seat Rated Load	159kg / 350lbs


INSTALLATION AND OPERATION INSTRUCTIONS

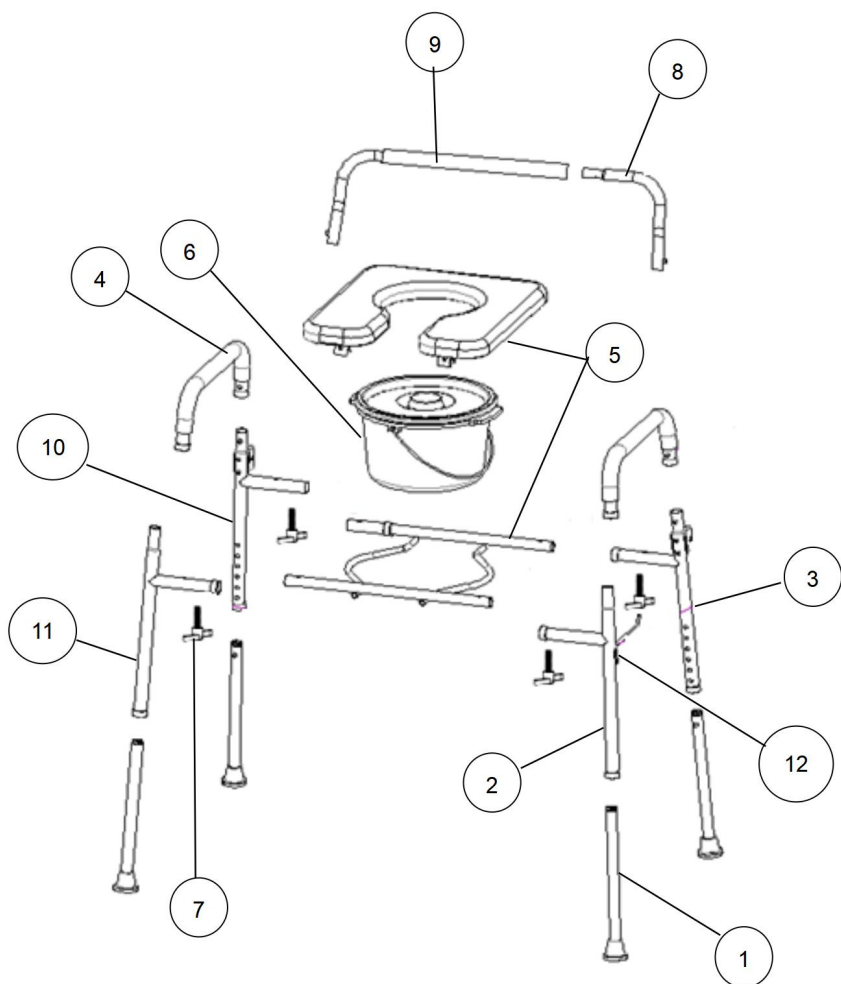


1. As shown in the figure, the four legs① are installed into the left front main frame②, the left rear main frame③, the right rear main frame⑩ and the right front main frame⑪ in turn.

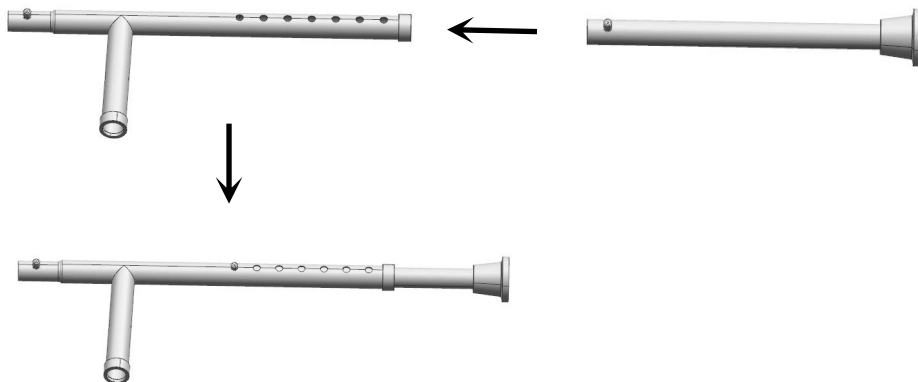


2. As shown in the figure, the assembled left front main frame ②, left rear main frame ③, right rear main frame ⑩, and right front main frame are put into the armrest tube ④ respectively, so that the marbles of each main frame eject normally.

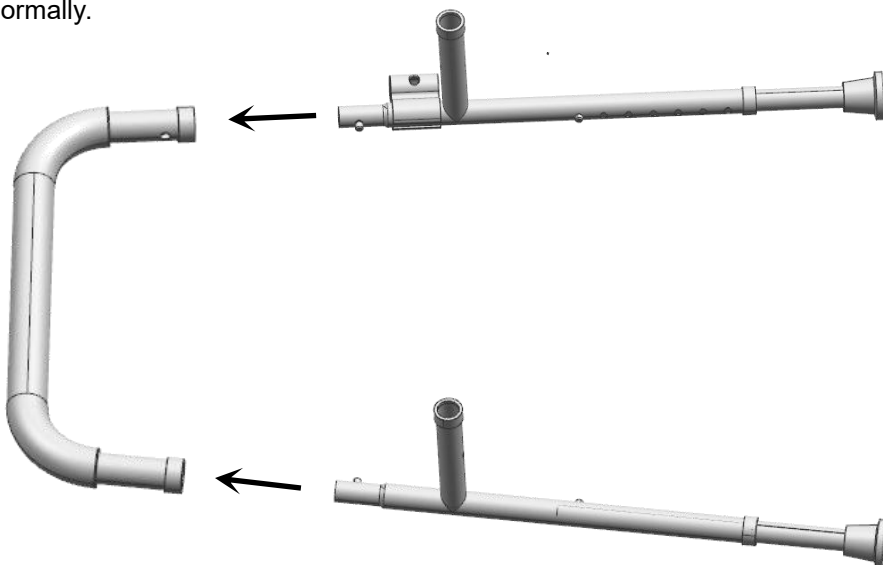


3. As shown in the figure, insert the assembled left and right main frames in line with the tube openings of the seat frame ⑤ (be careful not to install the seat frame and main frame in the front and rear directions in reverse).

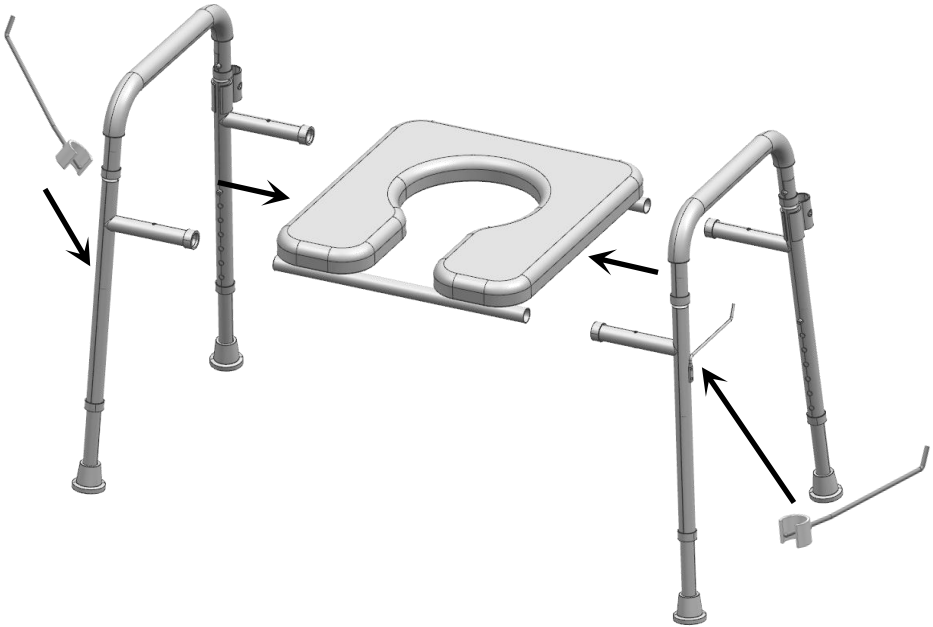


4. As shown in the figure, install the paper towel holder card ⑫ on the corresponding position of the left front main frame ② or right front main frame according to the usage habits.



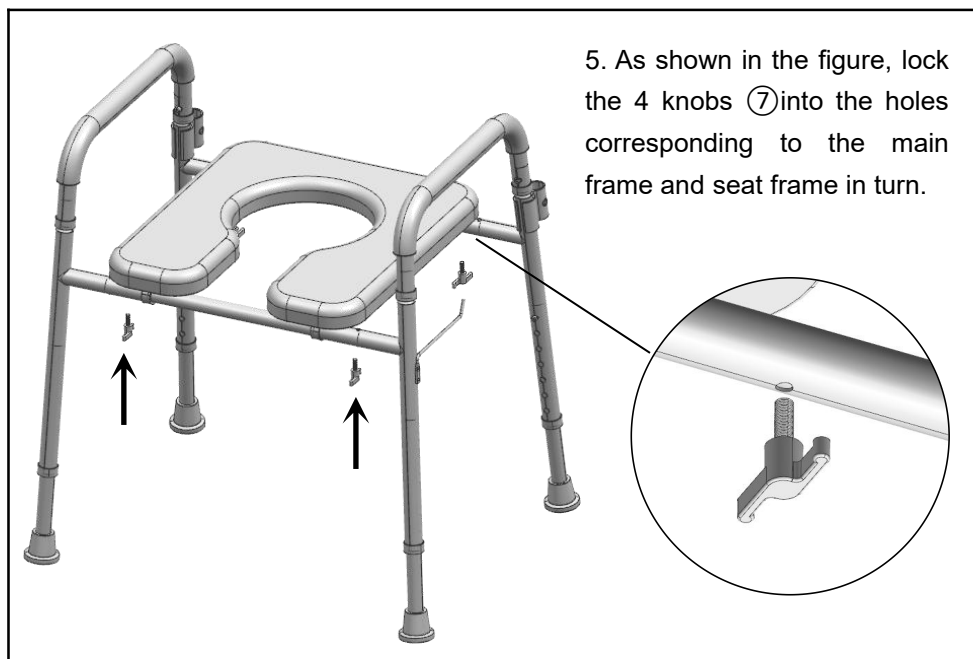


6. As shown in the figure, insert the short backrest tube ⑧ and the long backrest tube ⑨ mouth alignment, so that the marbles pop up normally (Note: Try to pull the two tubes apart by hand to confirm whether the two tubes are assembled).

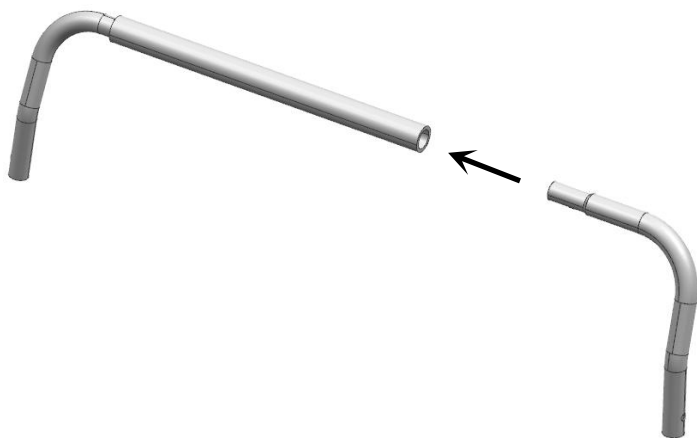

7. Insert the entire assembled backrest tube into the short tubes on either side of the rear main frame as shown.



8. As shown, lift the seat plate upwards and place the pail into the seat frame.

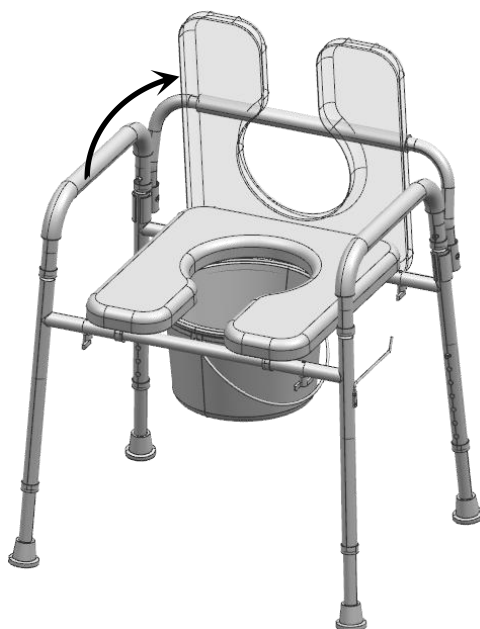

Zhongshan Bliss Medical Instrument Co., Ltd

Address: 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd
Unit 5 Albert Edward House,
The Pavilions Preston, United Kingdom
pooledas123@gmail.com
01772418127



SHUNSHUN GmbH
Römeräcker 9 Z2021,76351
Linkenheim-Hochstetten, Germany
euvertreter@gmail.com
+49 1727041930

Made In China

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate

www.vevor.com/support

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate www.vevor.com/support

COMMODE

MODEL:FBL730211

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

VEVOR[®]

TOUGH TOOLS, HALF PRICE

COMMODE

MODEL:FBL730211



NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

Technical Support and E-Warranty Certificate
www.vevor.com/support

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

WARNING:

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

Physiotherapist

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to standing position, place your hands on the rails firmly, and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).














IMPORTANT

1. Don't exceed the weight capacity max.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

SAVE THESE INSTRUCTION

PART LIST


When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.

NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Leg Tube	4	⑧		Short Backrest Tube	1
②		Left Front Main Frame	1	⑨		Long Backrest Tube	1
③		Left Rear Main Frame	1	⑩		Right Rear Main Frame	1
④		Armrest Tube	2	⑪		Right Front Main Frame	1
⑤		Seat	1	⑫		Paper Towel Holder	1
⑥		Pail & Splash Shield & Lid	1	⑬		Foot Mats (*Gifts)	2
⑦		Flat Knob	4				


PRODUCT PAREMETERS

Model	FBL730211
Seat Measures (L×W)	440×400mm / 17.3"×15.7"
Seat Height	495-645mm / 20.3"-25.4"
Seat Rated Load	159kg / 350lbs


INSTALLATION AND OPERATION INSTRUCTIONS

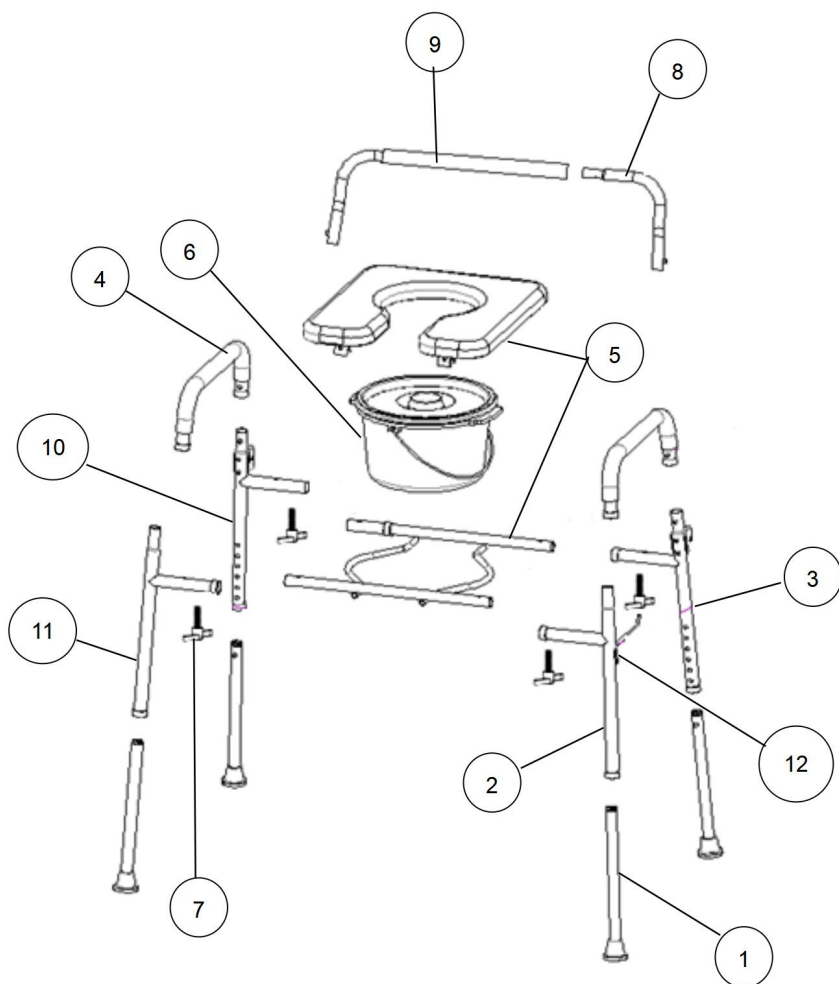


1. As shown in the figure, the four legs① are installed into the left front main frame②, the left rear main frame③, the right rear main frame⑩ and the right front main frame⑪ in turn.

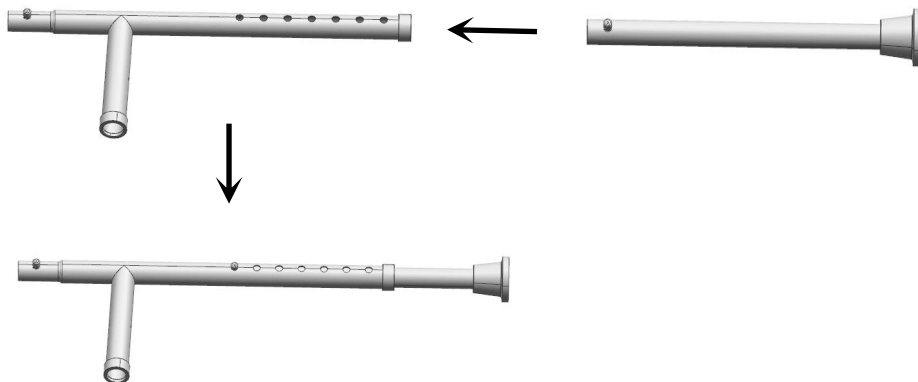


2. As shown in the figure, the assembled left front main frame ②, left rear main frame ③, right rear main frame ⑩, and right front main frame are put into the armrest tube ④ respectively, so that the marbles of each main frame eject normally.

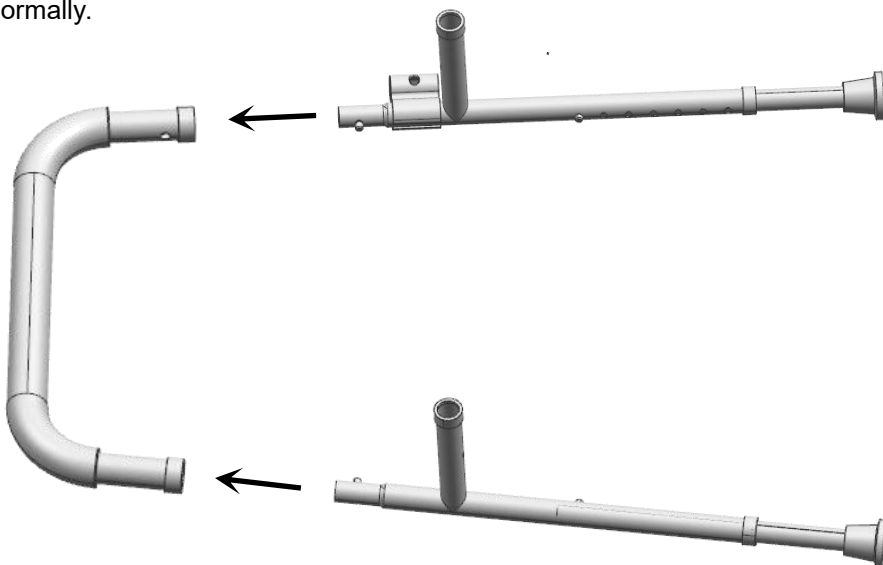


3. As shown in the figure, insert the assembled left and right main frames in line with the tube openings of the seat frame ⑤ (be careful not to install the seat frame and main frame in the front and rear directions in reverse).

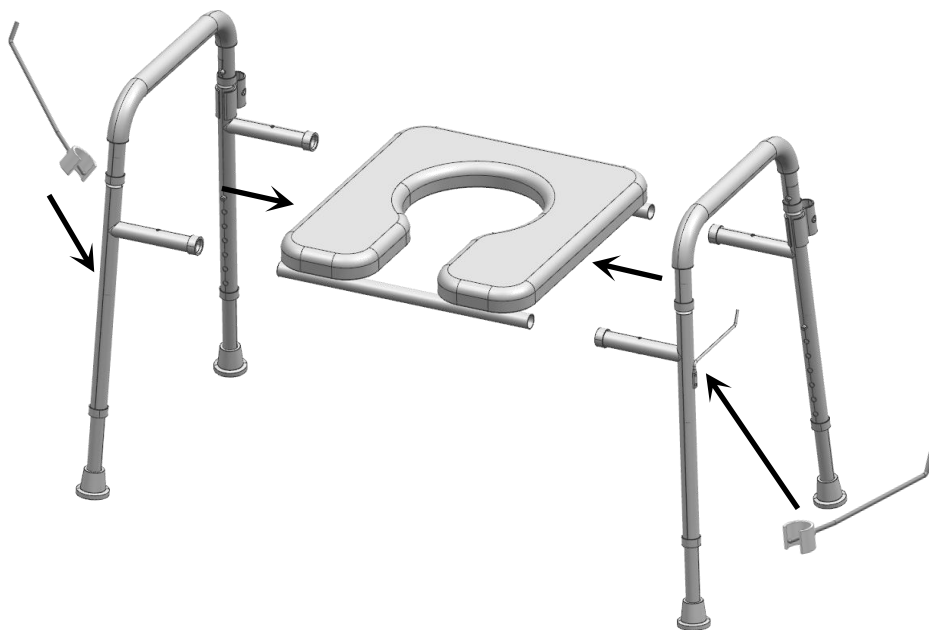


4. As shown in the figure, install the paper towel holder card ⑫ on the corresponding position of the left front main frame ② or right front main frame according to the usage habits.



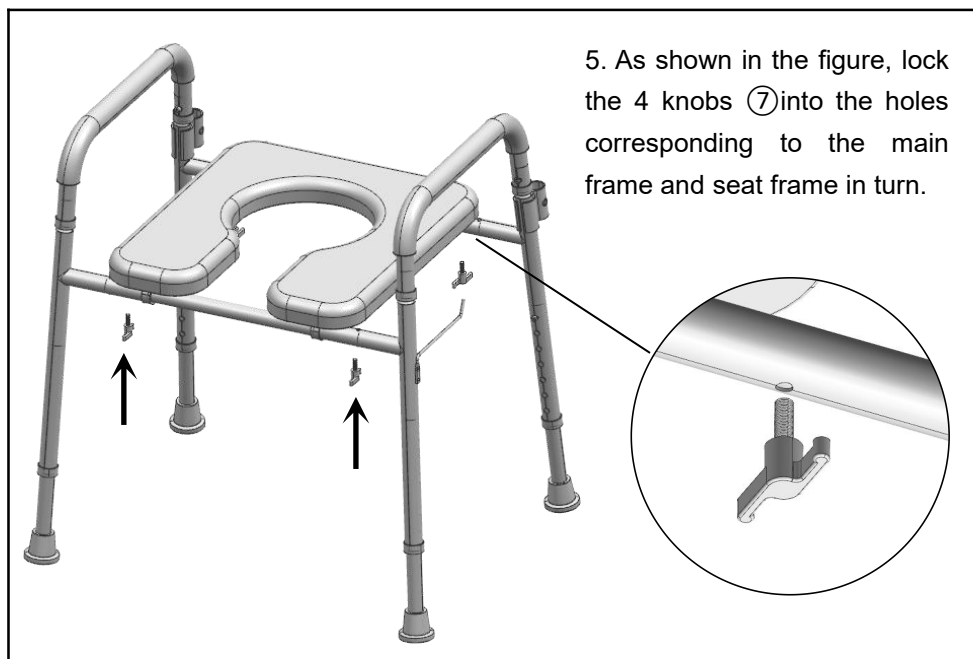


6. As shown in the figure, insert the short backrest tube ⑧ and the long backrest tube ⑨ mouth alignment, so that the marbles pop up normally (Note: Try to pull the two tubes apart by hand to confirm whether the two tubes are assembled).

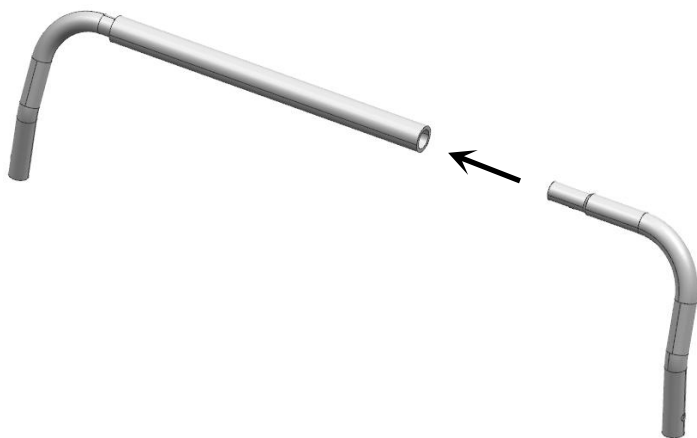

7. Insert the entire assembled backrest tube into the short tubes on either side of the rear main frame as shown.



8. As shown, lift the seat plate upwards and place the pail into the seat frame.

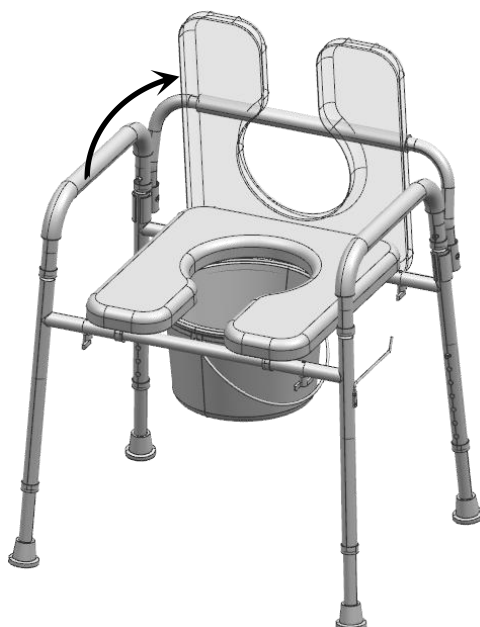

Zhongshan Bliss Medical Instrument Co., Ltd

Address: 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd
Unit 5 Albert Edward House,
The Pavilions Preston, United Kingdom
pooledas123@gmail.com
01772418127



SHUNSHUN GmbH
Römeräcker 9 Z2021,76351
Linkenheim-Hochstetten, Germany
euvertreter@gmail.com
+49 1727041930

Made In China

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate

www.vevor.com/support

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate www.vevor.com/support

COMMODE

MODEL:FBL730211

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

VEVOR[®]

TOUGH TOOLS, HALF PRICE

COMMODE

MODEL:FBL730211



NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

Technical Support and E-Warranty Certificate
www.vevor.com/support

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

WARNING:

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

Physiotherapist

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to standing position, place your hands on the rails firmly, and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).














IMPORTANT

1. Don't exceed the weight capacity max.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

SAVE THESE INSTRUCTION

PART LIST


When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.

NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Leg Tube	4	⑧		Short Backrest Tube	1
②		Left Front Main Frame	1	⑨		Long Backrest Tube	1
③		Left Rear Main Frame	1	⑩		Right Rear Main Frame	1
④		Armrest Tube	2	⑪		Right Front Main Frame	1
⑤		Seat	1	⑫		Paper Towel Holder	1
⑥		Pail & Splash Shield & Lid	1	⑬		Foot Mats (*Gifts)	2
⑦		Flat Knob	4				


PRODUCT PAREMETERS

Model	FBL730211
Seat Measures (L×W)	440×400mm / 17.3"×15.7"
Seat Height	495-645mm / 20.3"-25.4"
Seat Rated Load	159kg / 350lbs


INSTALLATION AND OPERATION INSTRUCTIONS

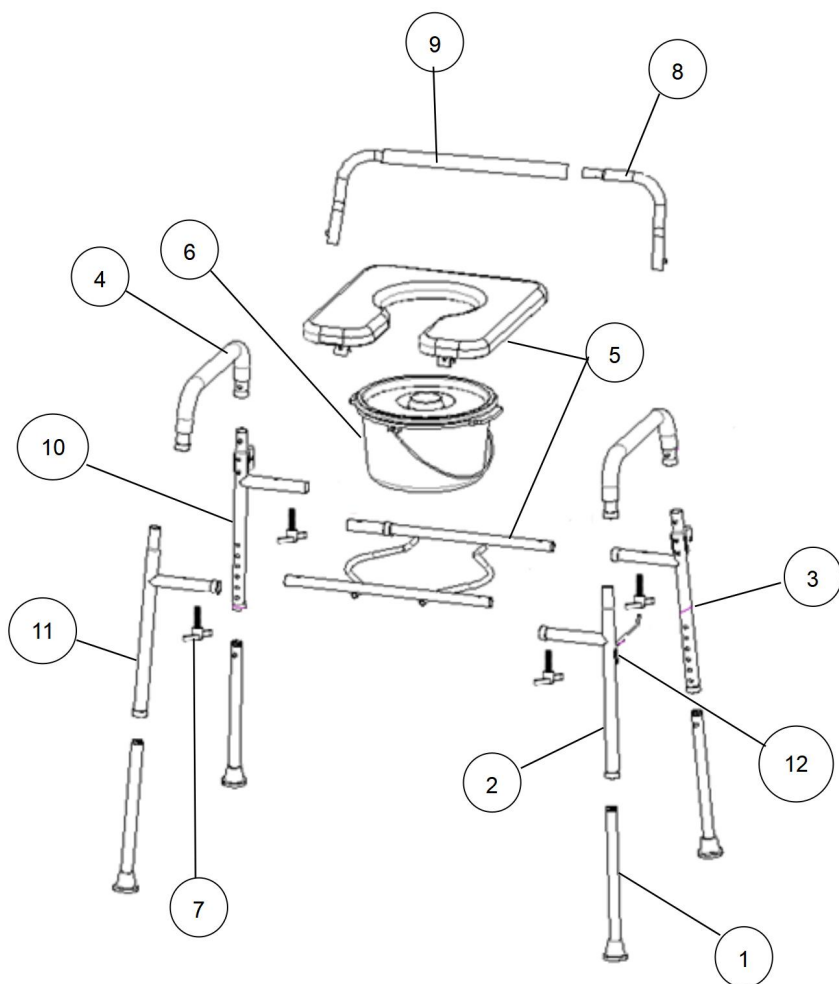


1. As shown in the figure, the four legs① are installed into the left front main frame②, the left rear main frame③, the right rear main frame⑩ and the right front main frame⑪ in turn.

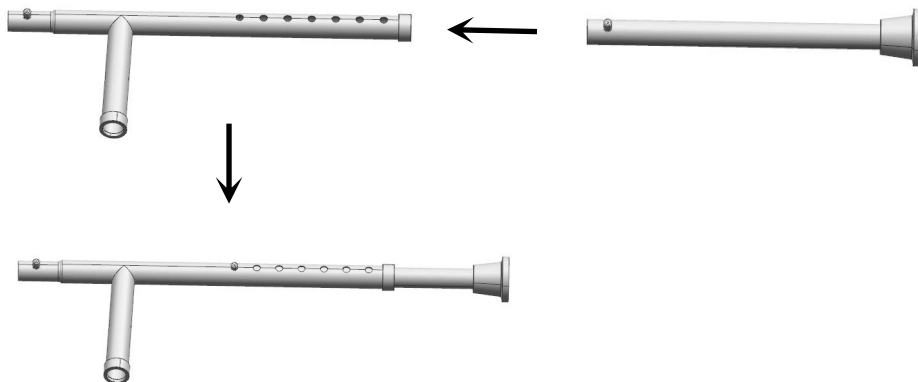


2. As shown in the figure, the assembled left front main frame ②, left rear main frame ③, right rear main frame ⑩, and right front main frame are put into the armrest tube ④ respectively, so that the marbles of each main frame eject normally.

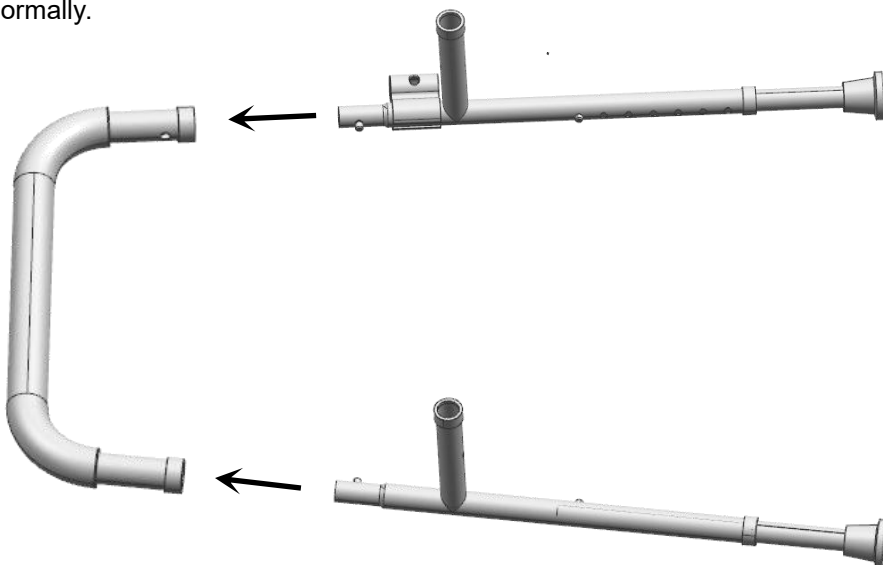


3. As shown in the figure, insert the assembled left and right main frames in line with the tube openings of the seat frame ⑤ (be careful not to install the seat frame and main frame in the front and rear directions in reverse).

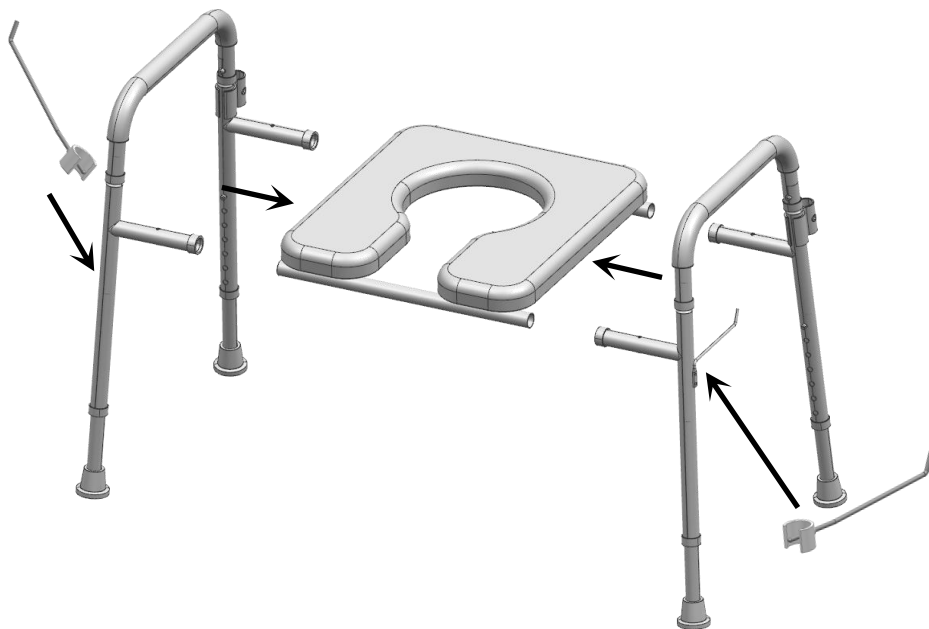


4. As shown in the figure, install the paper towel holder card ⑫ on the corresponding position of the left front main frame ② or right front main frame according to the usage habits.



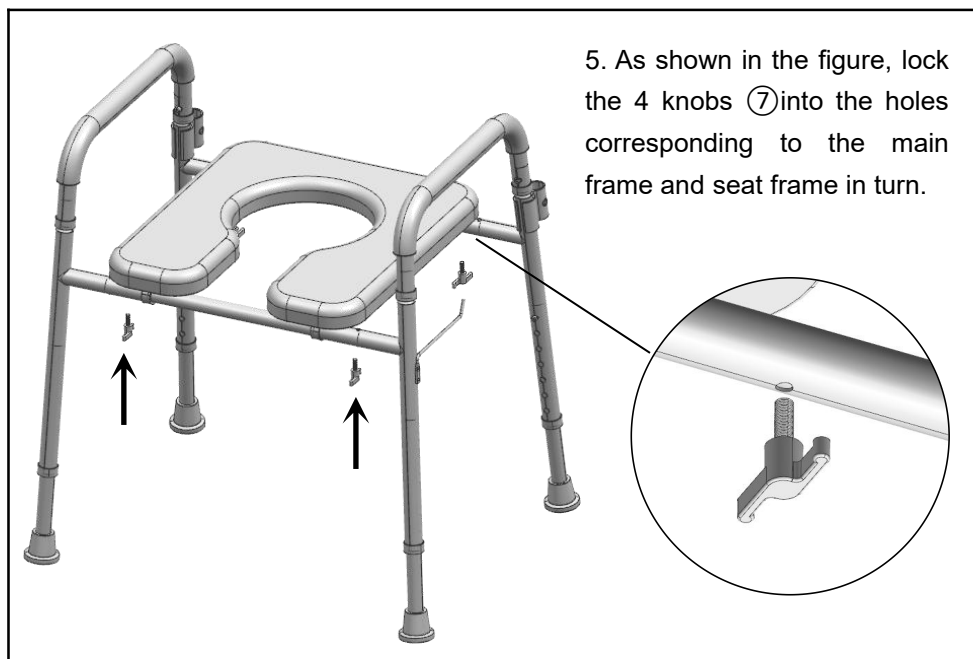


6. As shown in the figure, insert the short backrest tube ⑧ and the long backrest tube ⑨ mouth alignment, so that the marbles pop up normally (Note: Try to pull the two tubes apart by hand to confirm whether the two tubes are assembled).

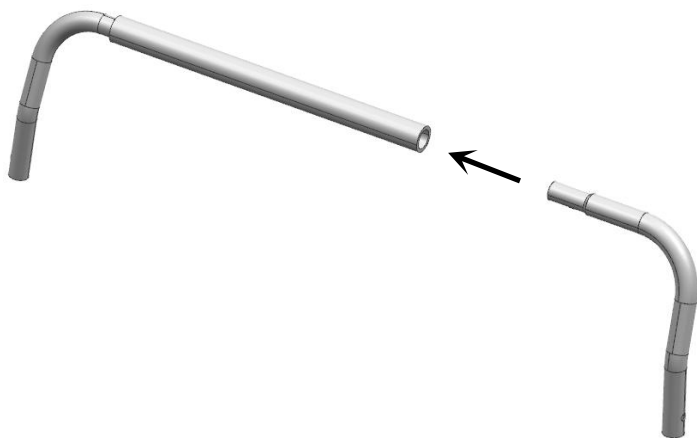

7. Insert the entire assembled backrest tube into the short tubes on either side of the rear main frame as shown.



8. As shown, lift the seat plate upwards and place the pail into the seat frame.

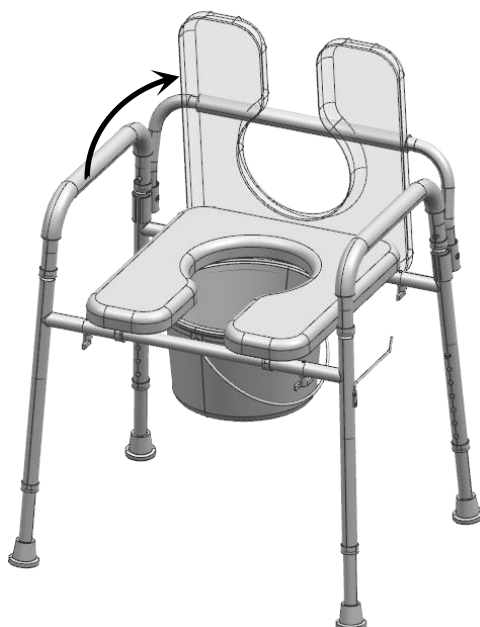

Zhongshan Bliss Medical Instrument Co., Ltd

Address: 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd
Unit 5 Albert Edward House,
The Pavilions Preston, United Kingdom
pooledas123@gmail.com
01772418127



SHUNSHUN GmbH
Römeräcker 9 Z2021,76351
Linkenheim-Hochstetten, Germany
euvertreter@gmail.com
+49 1727041930

Made In China

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate

www.vevor.com/support

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate www.vevor.com/support

COMMODE

MODEL:FBL730211

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

VEVOR[®]

TOUGH TOOLS, HALF PRICE

COMMODE

MODEL:FBL730211



NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

Technical Support and E-Warranty Certificate
www.vevor.com/support

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

WARNING:

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

Physiotherapist

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to standing position, place your hands on the rails firmly, and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).














IMPORTANT

1. Don't exceed the weight capacity max.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

SAVE THESE INSTRUCTION

PART LIST


When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.

NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Leg Tube	4	⑧		Short Backrest Tube	1
②		Left Front Main Frame	1	⑨		Long Backrest Tube	1
③		Left Rear Main Frame	1	⑩		Right Rear Main Frame	1
④		Armrest Tube	2	⑪		Right Front Main Frame	1
⑤		Seat	1	⑫		Paper Towel Holder	1
⑥		Pail & Splash Shield & Lid	1	⑬		Foot Mats (*Gifts)	2
⑦		Flat Knob	4				


PRODUCT PAREMETERS

Model	FBL730211
Seat Measures (L×W)	440×400mm / 17.3"×15.7"
Seat Height	495-645mm / 20.3"-25.4"
Seat Rated Load	159kg / 350lbs


INSTALLATION AND OPERATION INSTRUCTIONS

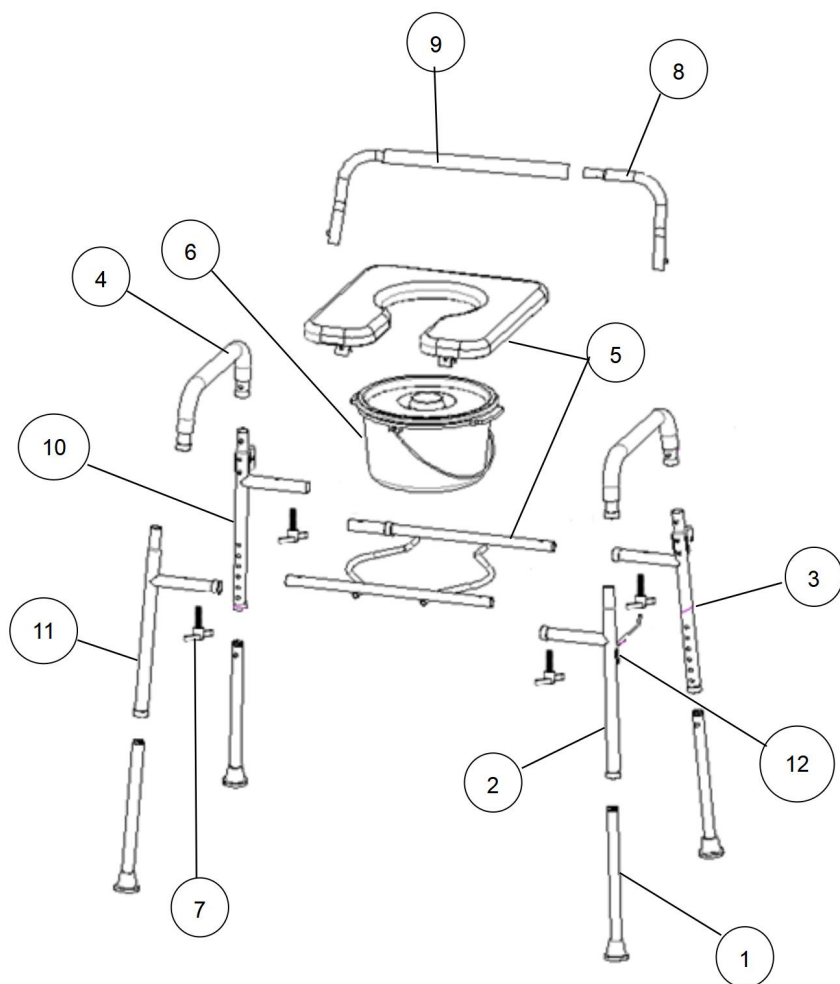


1. As shown in the figure, the four legs① are installed into the left front main frame②, the left rear main frame③, the right rear main frame⑩ and the right front main frame⑪ in turn.

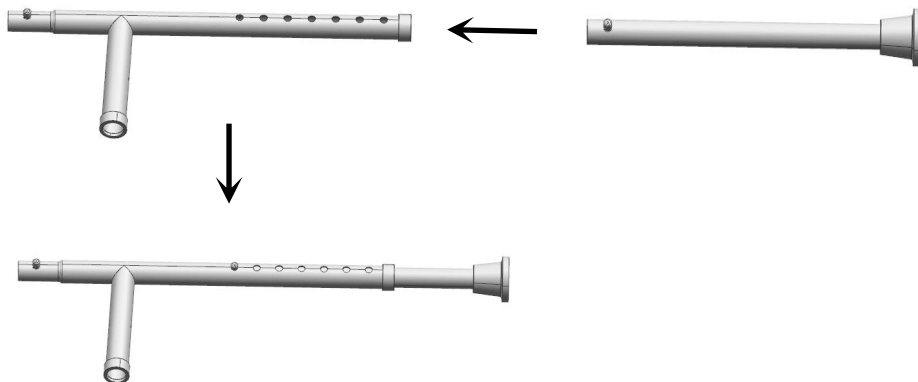


2. As shown in the figure, the assembled left front main frame ②, left rear main frame ③, right rear main frame ⑩, and right front main frame are put into the armrest tube ④ respectively, so that the marbles of each main frame eject normally.

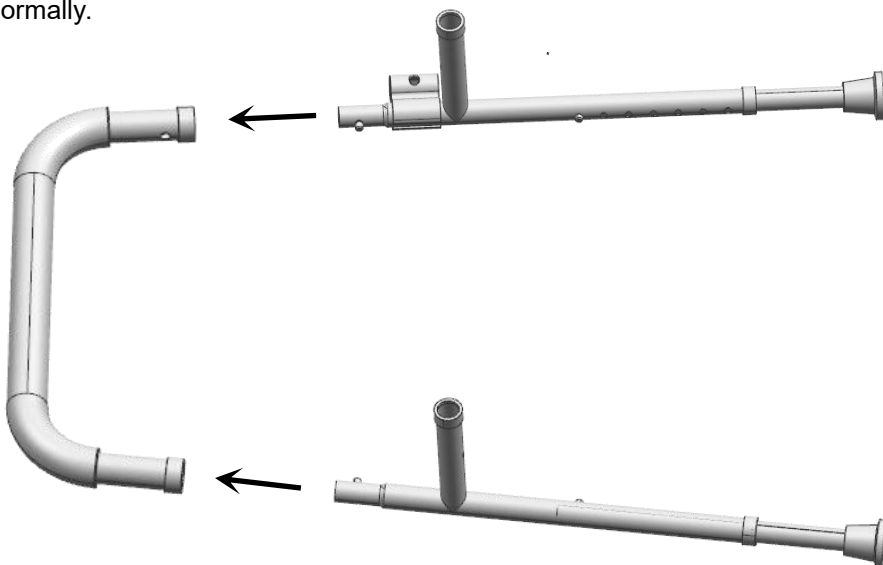


3. As shown in the figure, insert the assembled left and right main frames in line with the tube openings of the seat frame ⑤ (be careful not to install the seat frame and main frame in the front and rear directions in reverse).

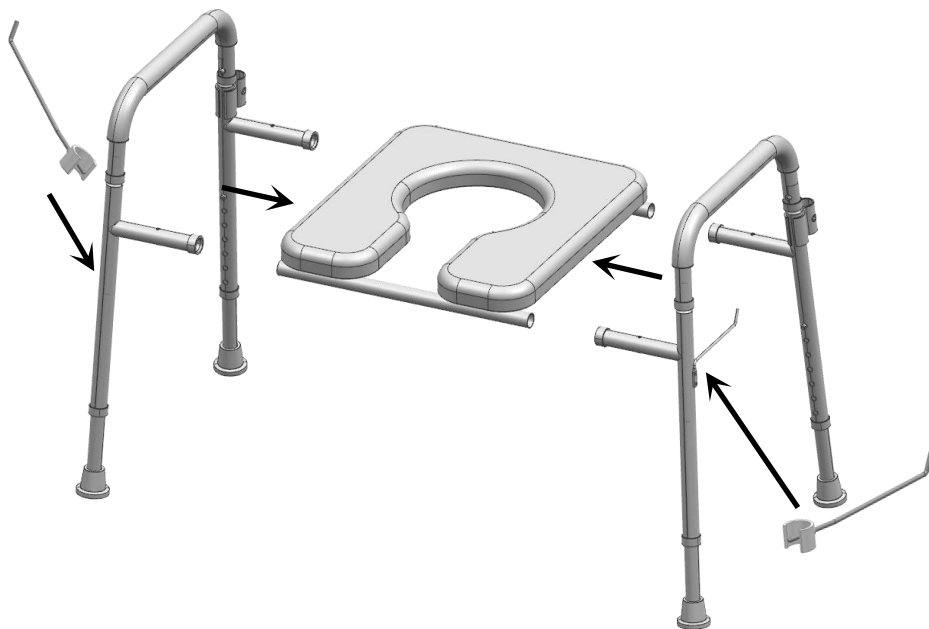


4. As shown in the figure, install the paper towel holder card ⑫ on the corresponding position of the left front main frame ② or right front main frame according to the usage habits.



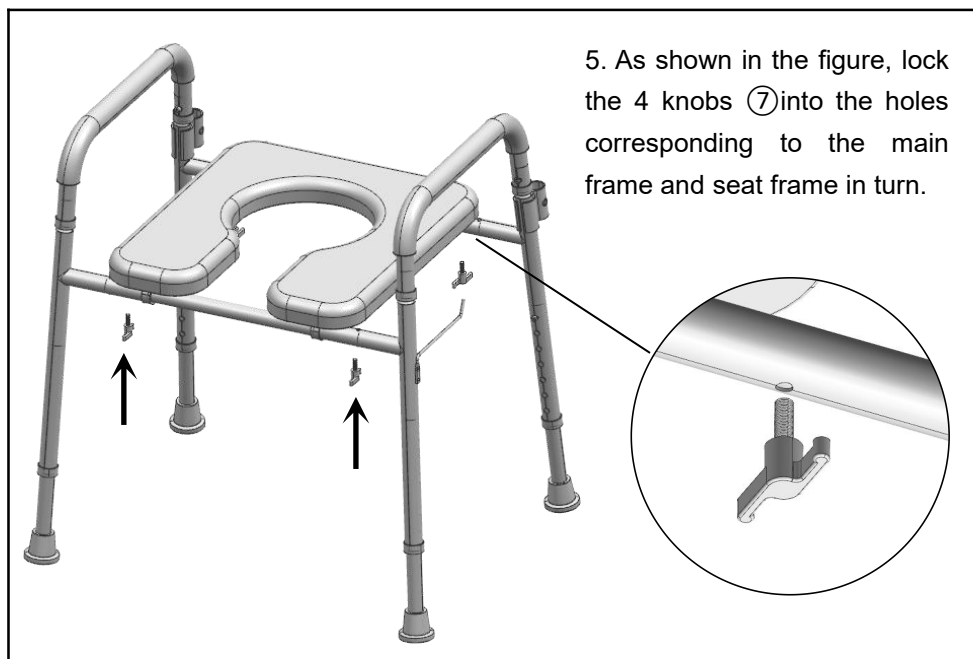


6. As shown in the figure, insert the short backrest tube ⑧ and the long backrest tube ⑨ mouth alignment, so that the marbles pop up normally (Note: Try to pull the two tubes apart by hand to confirm whether the two tubes are assembled).

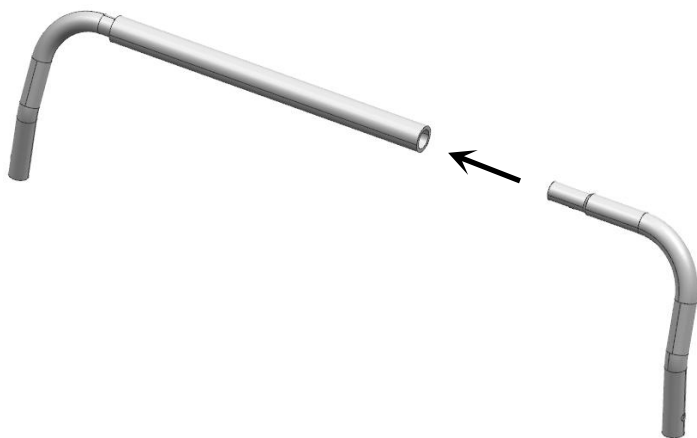

7. Insert the entire assembled backrest tube into the short tubes on either side of the rear main frame as shown.



8. As shown, lift the seat plate upwards and place the pail into the seat frame.

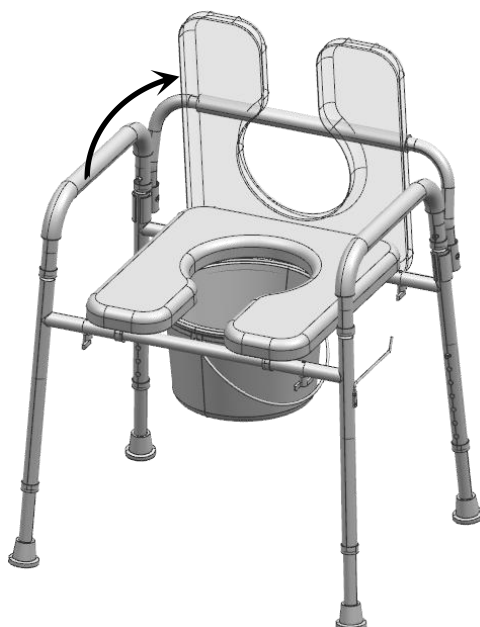

Zhongshan Bliss Medical Instrument Co., Ltd

Address: 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd
Unit 5 Albert Edward House,
The Pavilions Preston, United Kingdom
pooledas123@gmail.com
01772418127



SHUNSHUN GmbH
Römeräcker 9 Z2021,76351
Linkenheim-Hochstetten, Germany
euvertreter@gmail.com
+49 1727041930

Made In China

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate

www.vevor.com/support

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate www.vevor.com/support

COMMODE

MODEL:FBL730211

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

VEVOR[®]

TOUGH TOOLS, HALF PRICE

COMMODE

MODEL:FBL730211



NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

Technical Support and E-Warranty Certificate
www.vevor.com/support

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

WARNING:

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

Physiotherapist

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to standing position, place your hands on the rails firmly, and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).














IMPORTANT

1. Don't exceed the weight capacity max.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

SAVE THESE INSTRUCTION

PART LIST


When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.

NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Leg Tube	4	⑧		Short Backrest Tube	1
②		Left Front Main Frame	1	⑨		Long Backrest Tube	1
③		Left Rear Main Frame	1	⑩		Right Rear Main Frame	1
④		Armrest Tube	2	⑪		Right Front Main Frame	1
⑤		Seat	1	⑫		Paper Towel Holder	1
⑥		Pail & Splash Shield & Lid	1	⑬		Foot Mats (*Gifts)	2
⑦		Flat Knob	4				


PRODUCT PAREMETERS

Model	FBL730211
Seat Measures (L×W)	440×400mm / 17.3"×15.7"
Seat Height	495-645mm / 20.3"-25.4"
Seat Rated Load	159kg / 350lbs


INSTALLATION AND OPERATION INSTRUCTIONS

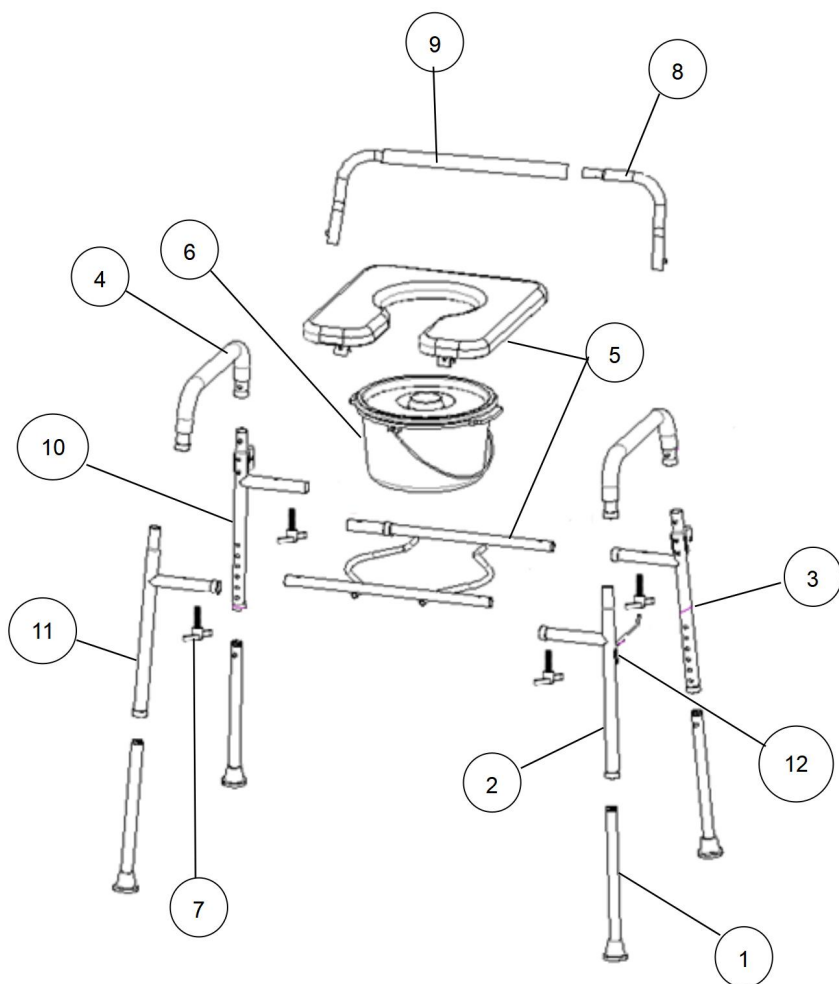


1. As shown in the figure, the four legs① are installed into the left front main frame②, the left rear main frame③, the right rear main frame⑩ and the right front main frame⑪ in turn.

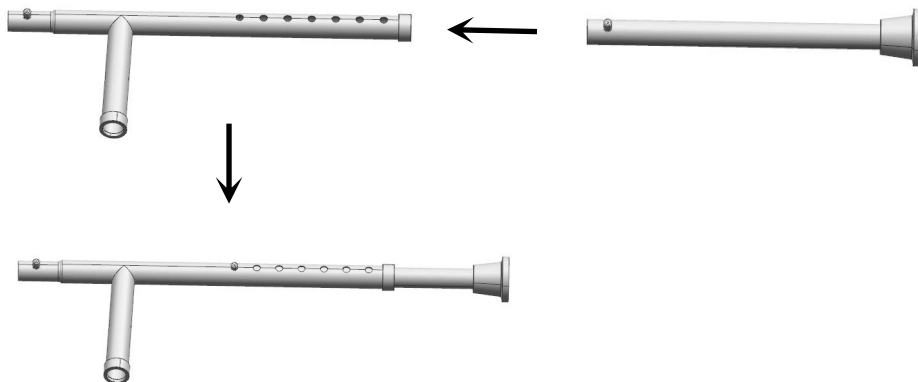


2. As shown in the figure, the assembled left front main frame ②, left rear main frame ③, right rear main frame ⑩, and right front main frame are put into the armrest tube ④ respectively, so that the marbles of each main frame eject normally.

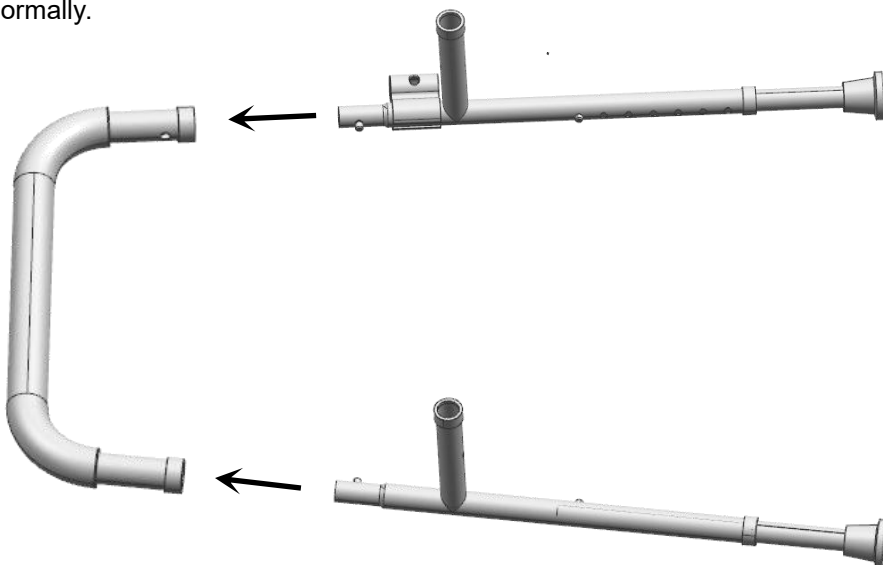


3. As shown in the figure, insert the assembled left and right main frames in line with the tube openings of the seat frame ⑤ (be careful not to install the seat frame and main frame in the front and rear directions in reverse).

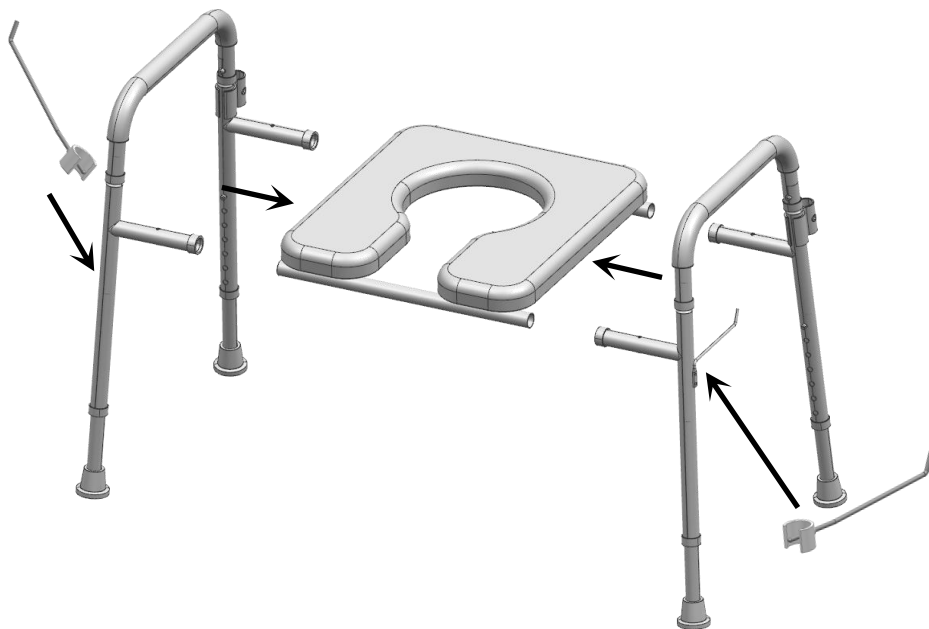


4. As shown in the figure, install the paper towel holder card ⑫ on the corresponding position of the left front main frame ② or right front main frame according to the usage habits.



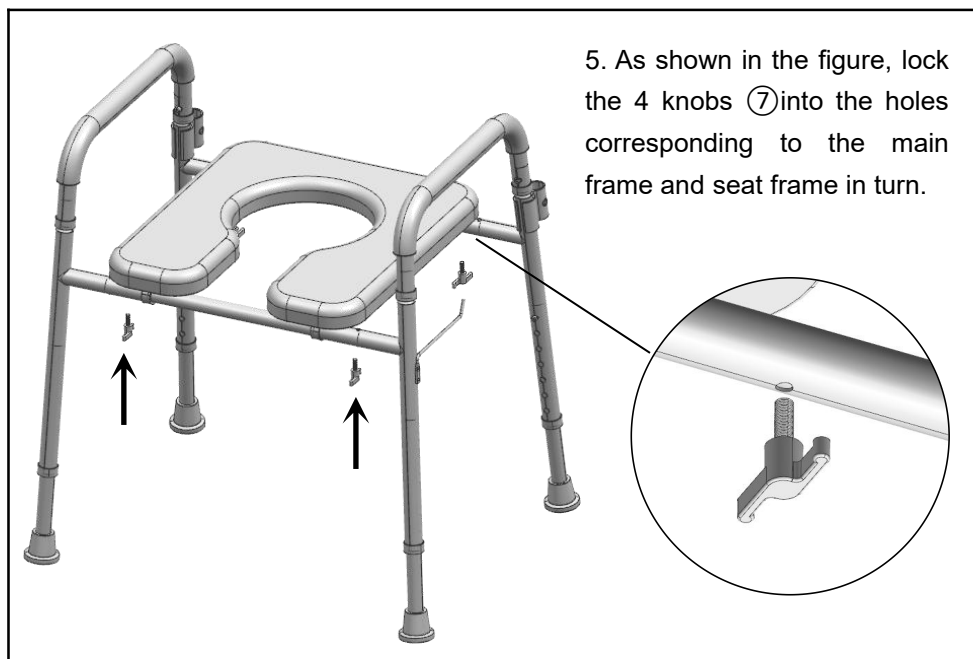


6. As shown in the figure, insert the short backrest tube ⑧ and the long backrest tube ⑨ mouth alignment, so that the marbles pop up normally (Note: Try to pull the two tubes apart by hand to confirm whether the two tubes are assembled).

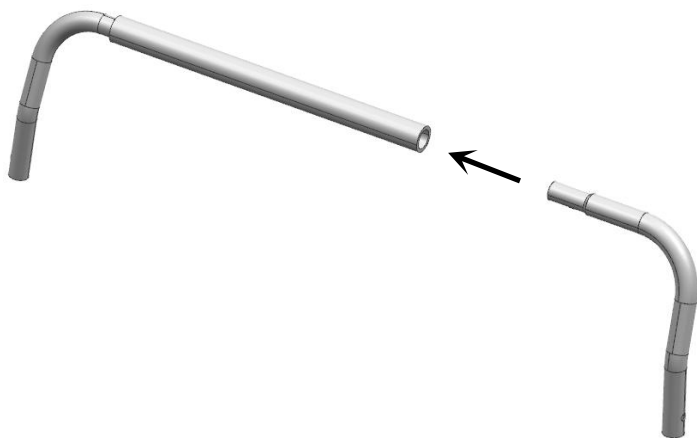

7. Insert the entire assembled backrest tube into the short tubes on either side of the rear main frame as shown.



8. As shown, lift the seat plate upwards and place the pail into the seat frame.

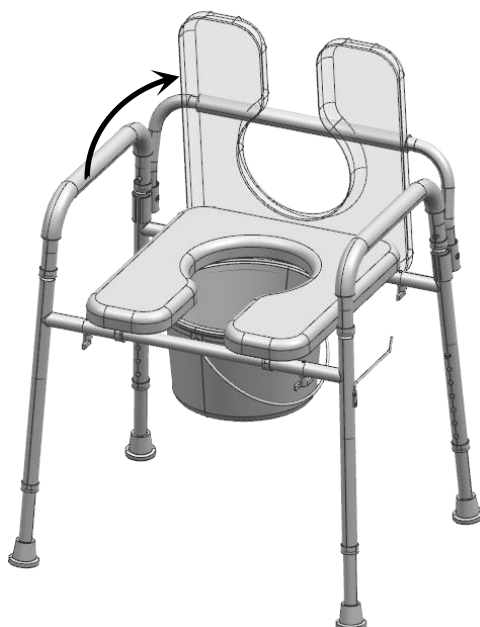

Zhongshan Bliss Medical Instrument Co., Ltd

Address: 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd
Unit 5 Albert Edward House,
The Pavilions Preston, United Kingdom
pooledas123@gmail.com
01772418127



SHUNSHUN GmbH
Römeräcker 9 Z2021,76351
Linkenheim-Hochstetten, Germany
euvertreter@gmail.com
+49 1727041930

Made In China

VEVOR[®]

TOUGH TOOLS, HALF PRICE

Technical Support and E-Warranty Certificate

www.vevor.com/support